

SUPERVISOR TEST




SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 05/10/2021

OPERATOR NAME:
 ANDREW S COLE-HATCHARD
 Permit #: 47565
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:58
INTERNAL STANDARD	VERIFIED	09:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:59
BLANK TEST	0.00	10:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:00
BLANK TEST	0.00	10:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:01
BLANK TEST	0.00	10:02

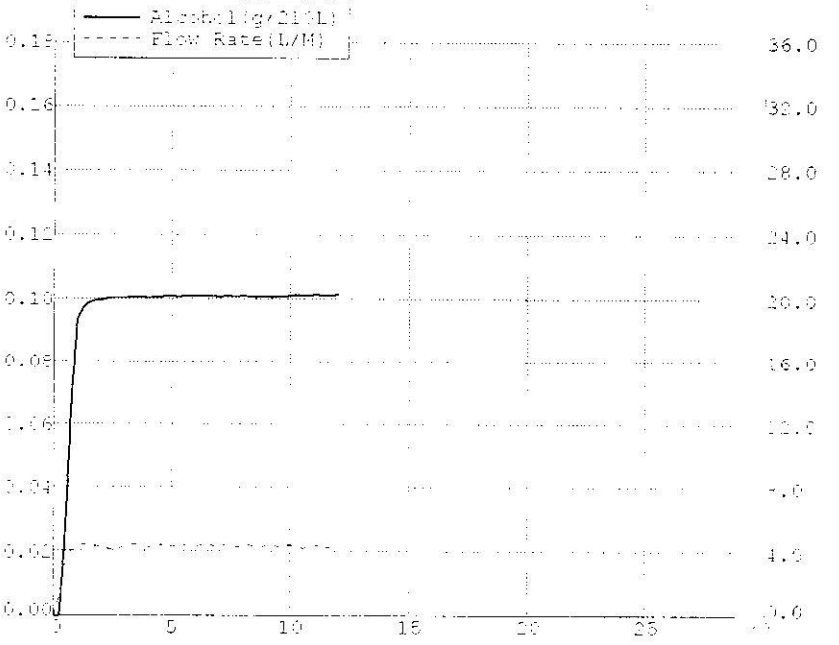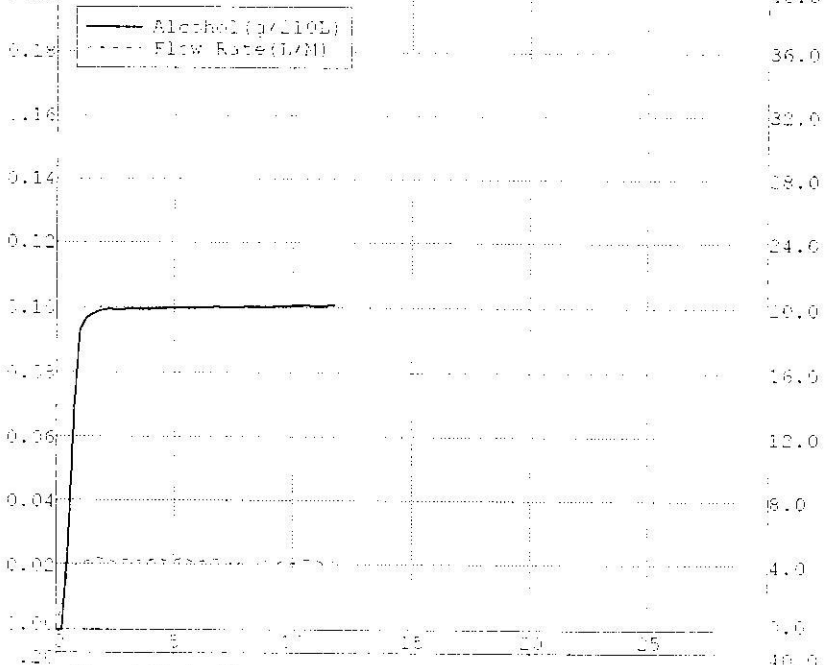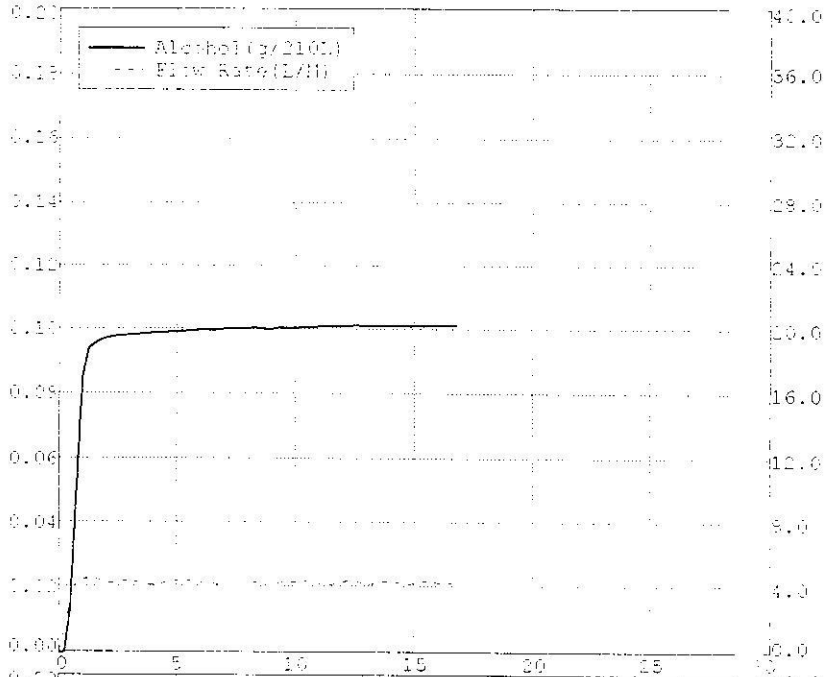

8πÅÇ!FD!▼CÇ