

SOLUTION CHANGE




SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 08/06/2021

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:13
INTERNAL STANDARD	VERIFIED	11:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:13
BLANK TEST	0.00	11:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:15
BLANK TEST	0.00	11:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:16
BLANK TEST	0.00	11:17

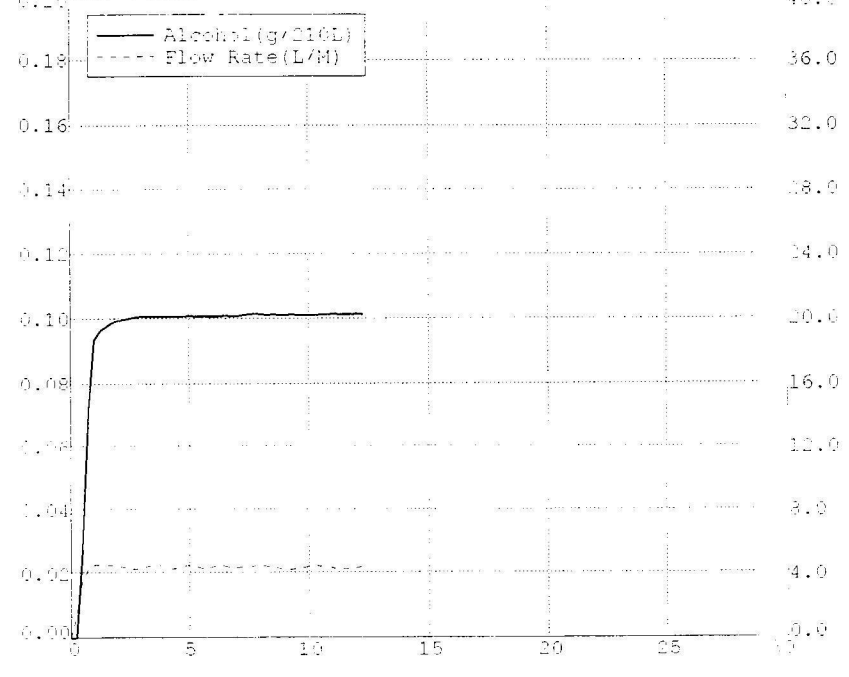

MA 614

