

SOLUTION CHANGE




SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 09/01/2021

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:02
INTERNAL STANDARD	VERIFIED	13:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:03
BLANK TEST	0.00	13:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:04
BLANK TEST	0.00	13:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:05
BLANK TEST	0.00	13:06

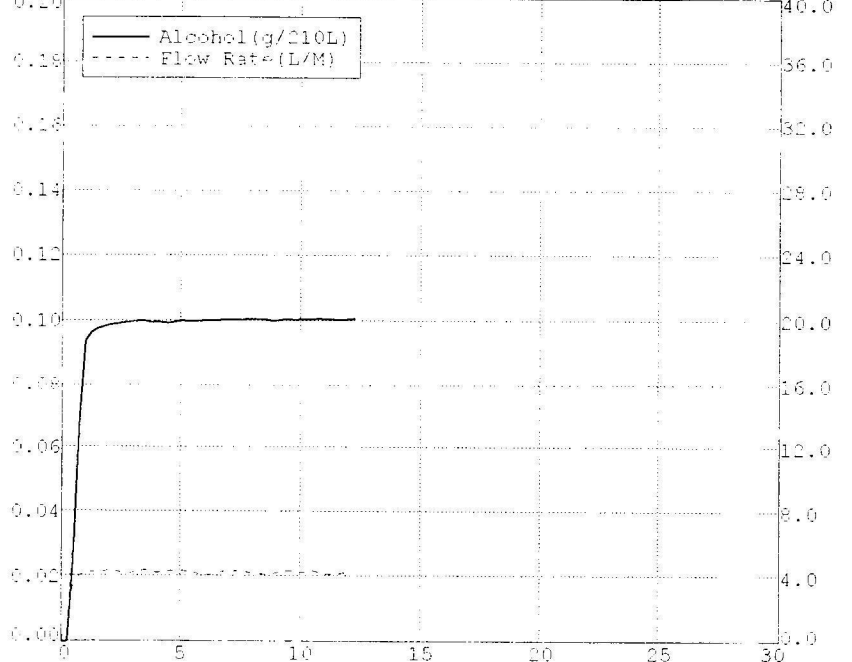

614

