

SUPERVISOR TEST




-----  
 SPRING VALLEY VILLAGE  
 POLICE DEPT  
 DATAMASTER dmt: 127106  
 -----

Date: 09/18/2021

OPERATOR NAME:  
 BRANDON KING  
 Permit #: 36388  
 Operator Agency/Dept: SPRING VALLEY PD  
 Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:13
INTERNAL STANDARD	VERIFIED	09:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:13
BLANK TEST	0.00	09:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:15
BLANK TEST	0.00	09:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:16
BLANK TEST	0.00	09:17

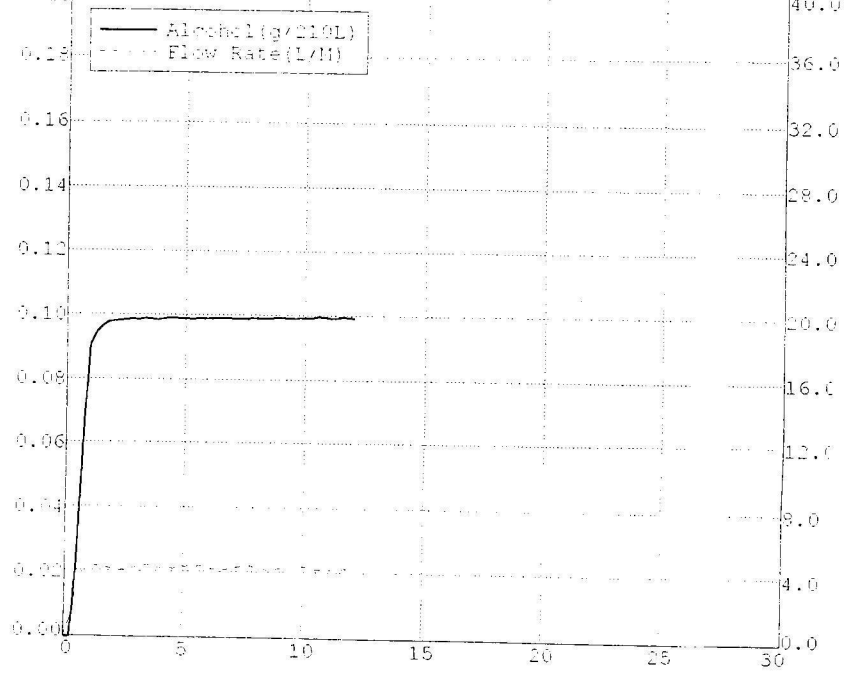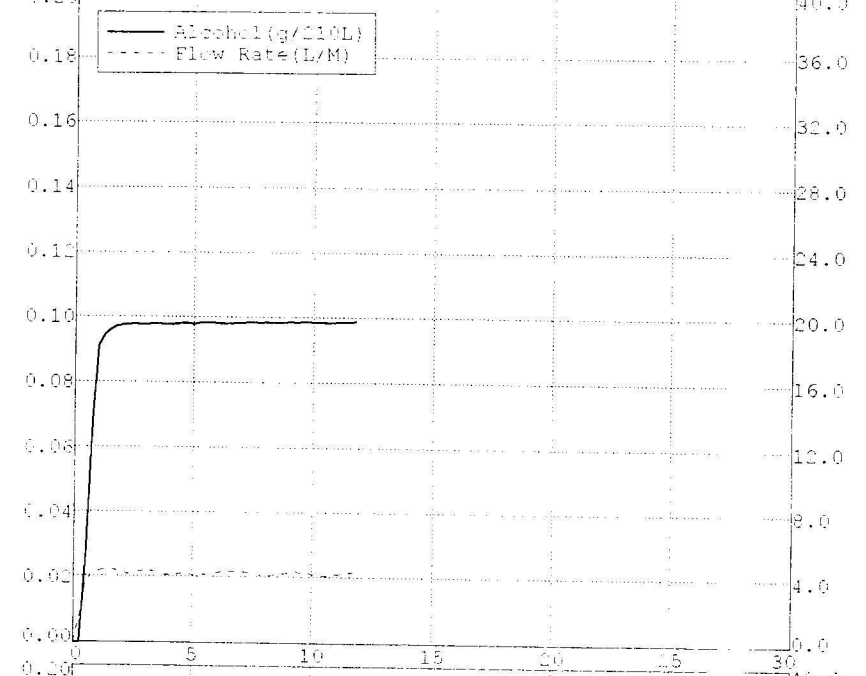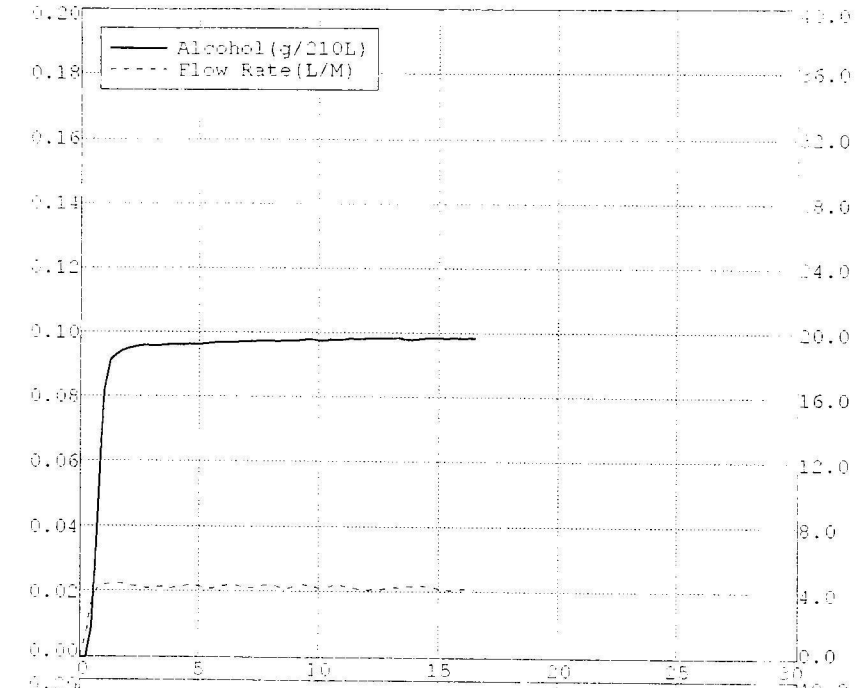

614