

SOLUTION CHANGE




SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 11/01/2021

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:23
INTERNAL STANDARD	VERIFIED	11:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:24
BLANK TEST	0.00	11:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:25
BLANK TEST	0.00	11:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:26
BLANK TEST	0.00	11:27

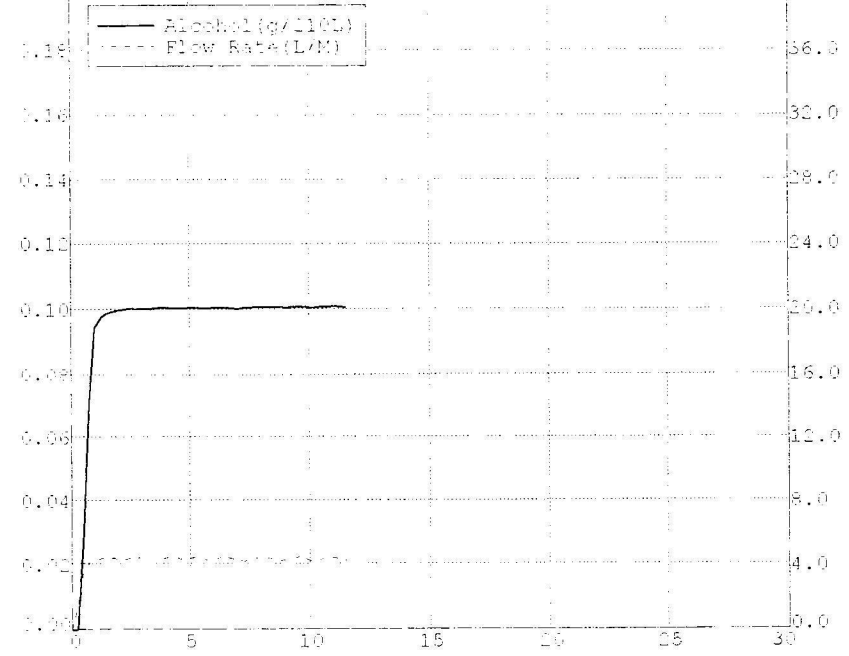

0614

