

SOLUTION CHANGE




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 01/03/2022

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:29
INTERNAL STANDARD	VERIFIED	02:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:30
BLANK TEST	0.00	02:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:31
BLANK TEST	0.00	02:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:32
BLANK TEST	0.00	02:33

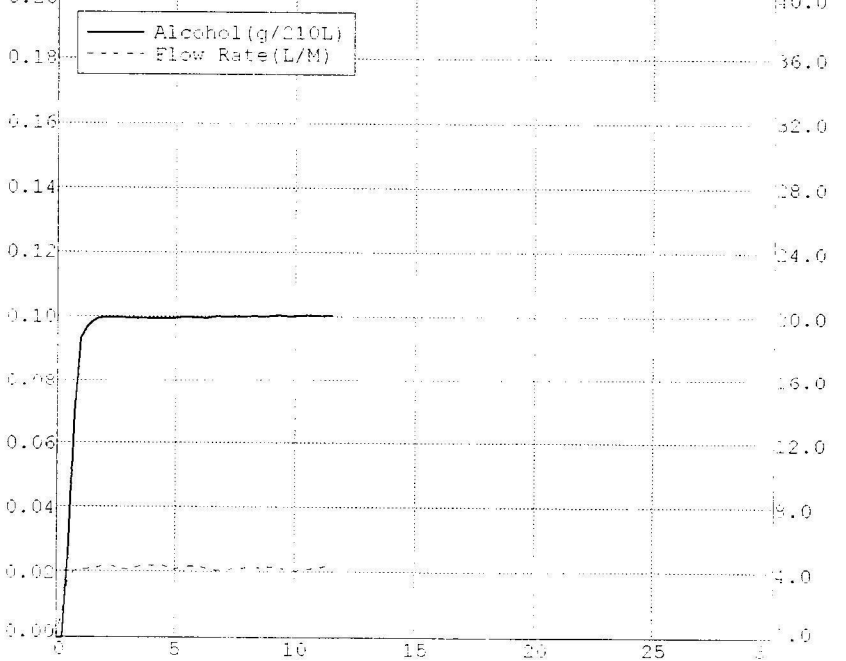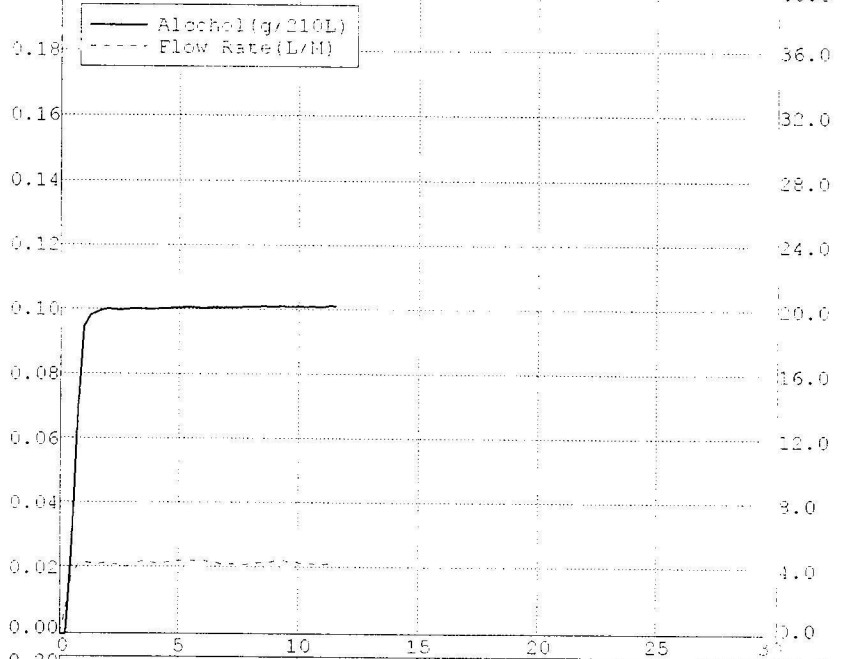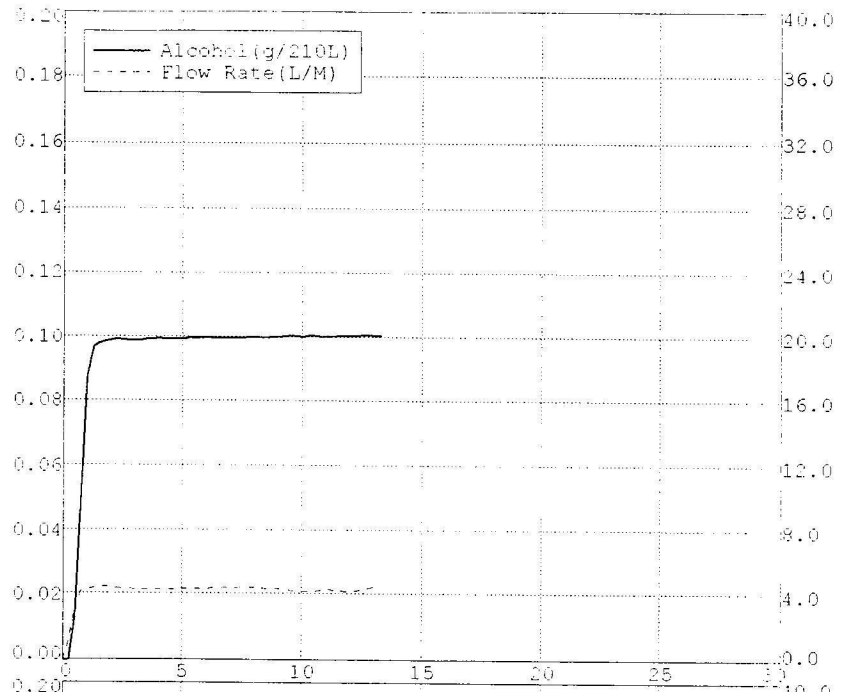

0614

