

SUPERVISOR TEST




SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 02/08/2022

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:45
INTERNAL STANDARD	VERIFIED	16:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:45
BLANK TEST	0.00	16:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:47
BLANK TEST	0.00	16:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:48
BLANK TEST	0.00	16:49

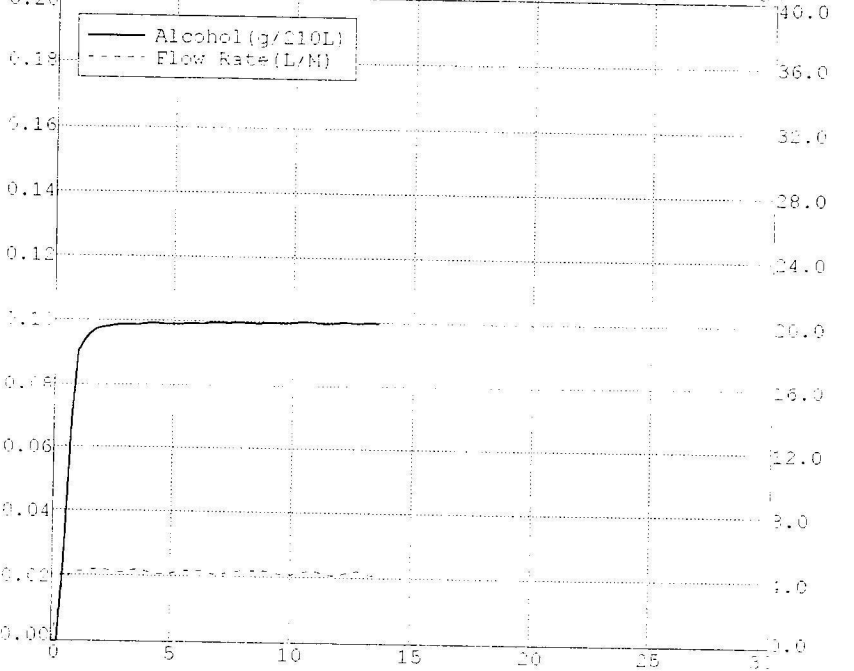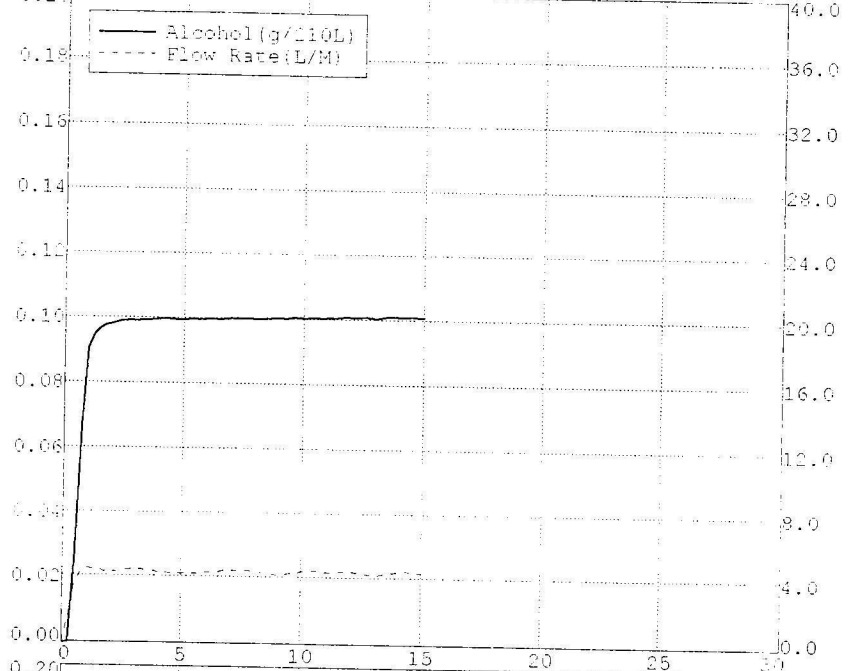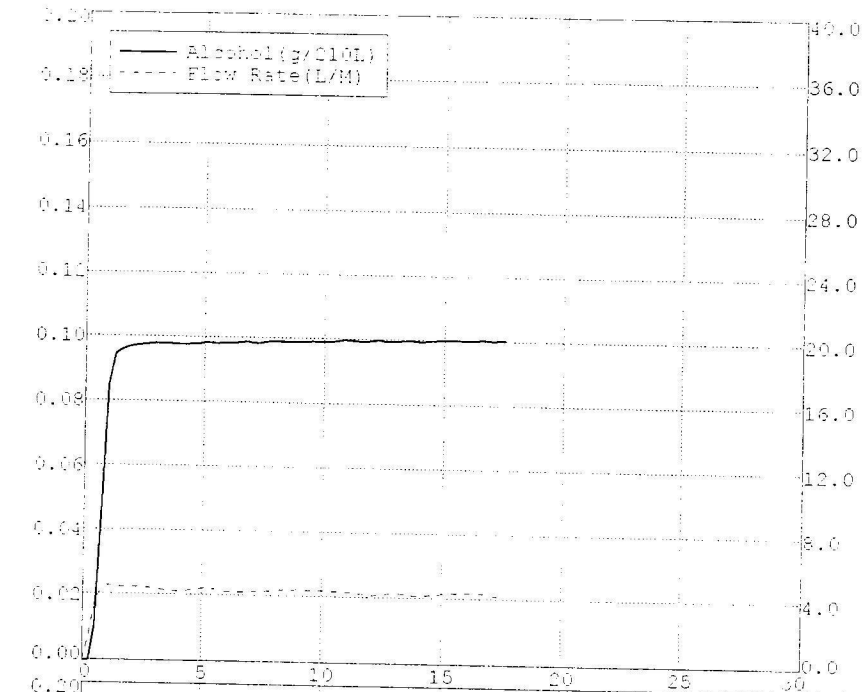

614