

SUPERVISOR TEST




SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 02/15/2022

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:50
INTERNAL STANDARD	VERIFIED	13:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:50
BLANK TEST	0.00	13:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:51
BLANK TEST	0.00	13:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:53
BLANK TEST	0.00	13:53

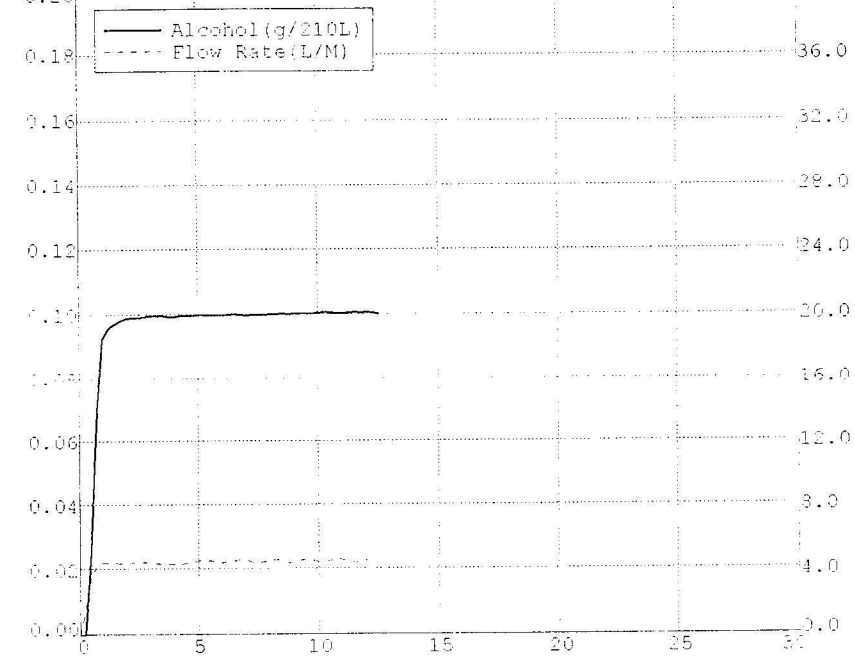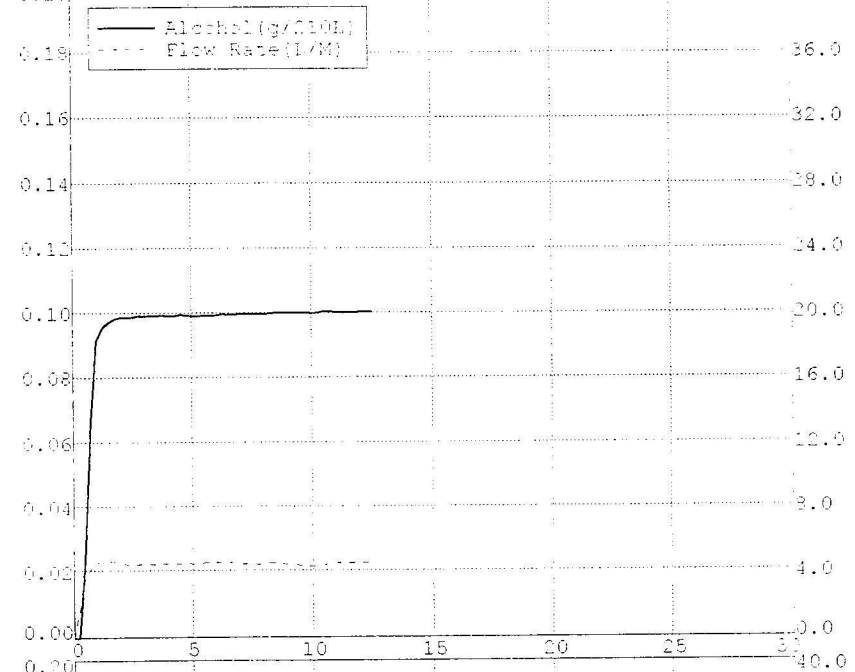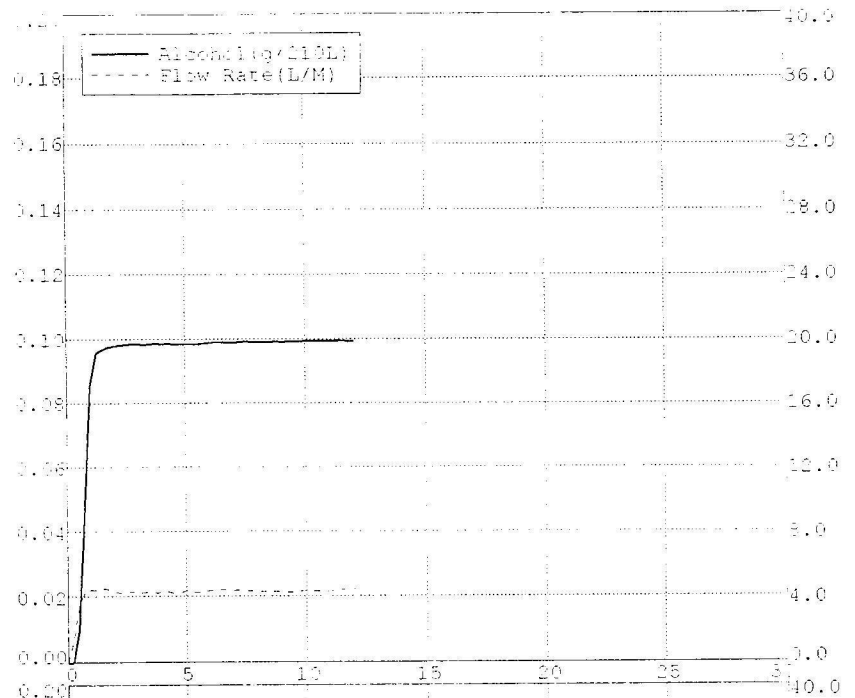

Handwritten signature/initials: @ 614