

SOLUTION CHANGE




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 02/17/2022

OPERATOR NAME:
ELYOKEM G UNGAR
Permit #: 45754
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:21
INTERNAL STANDARD	VERIFIED	16:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:22
BLANK TEST	0.00	16:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:23
BLANK TEST	0.00	16:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:24
BLANK TEST	0.00	16:25

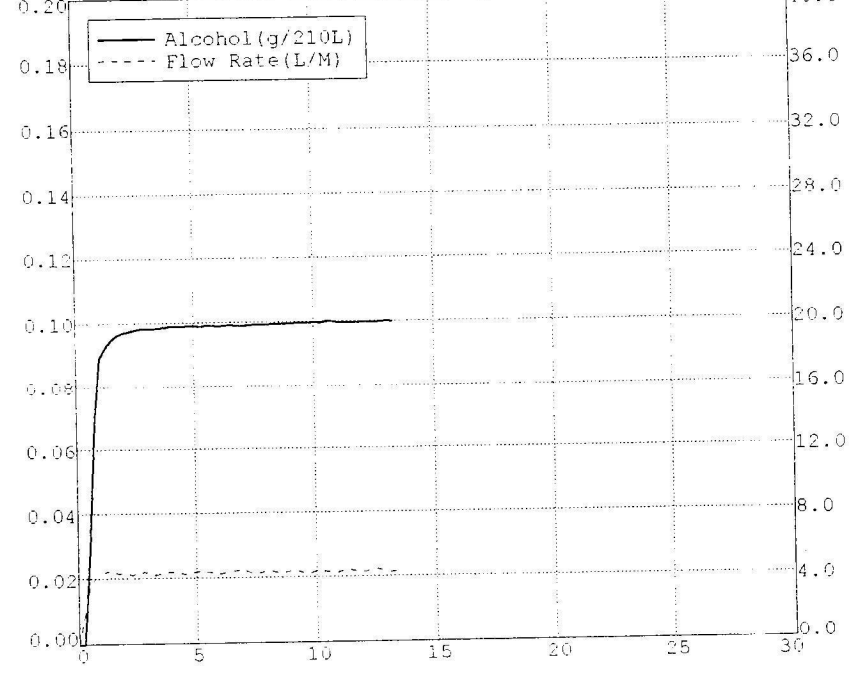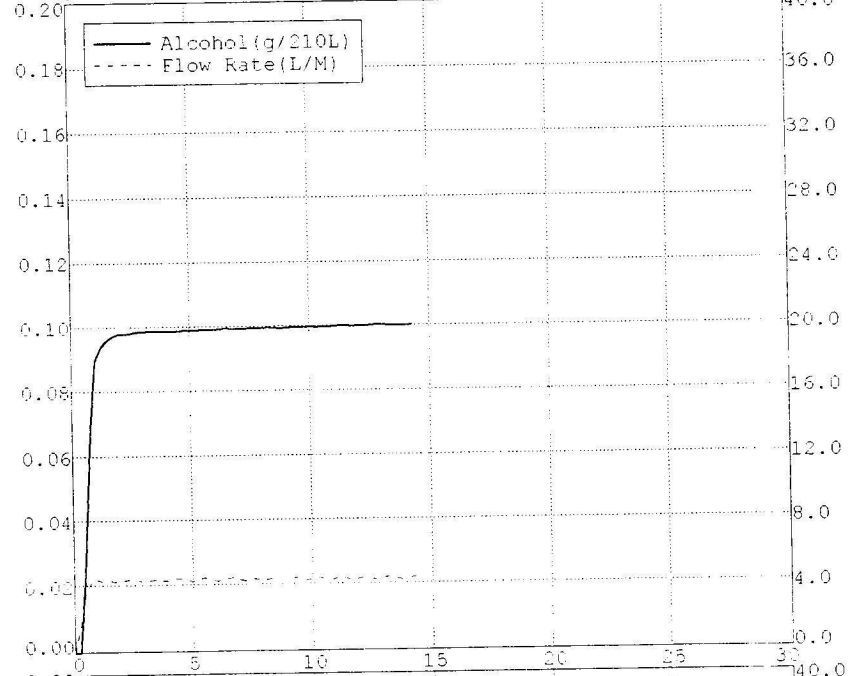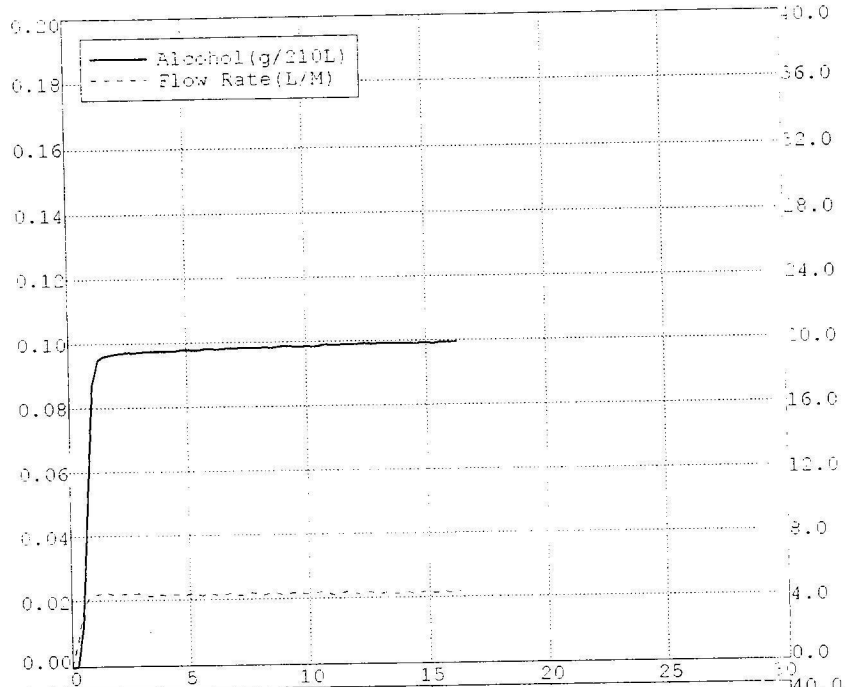

B. #12 391

