

SUPERVISOR TEST




SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 02/28/2022

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:15
INTERNAL STANDARD	VERIFIED	08:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:16
BLANK TEST	0.00	08:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:17
BLANK TEST	0.00	08:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:18
BLANK TEST	0.00	08:19

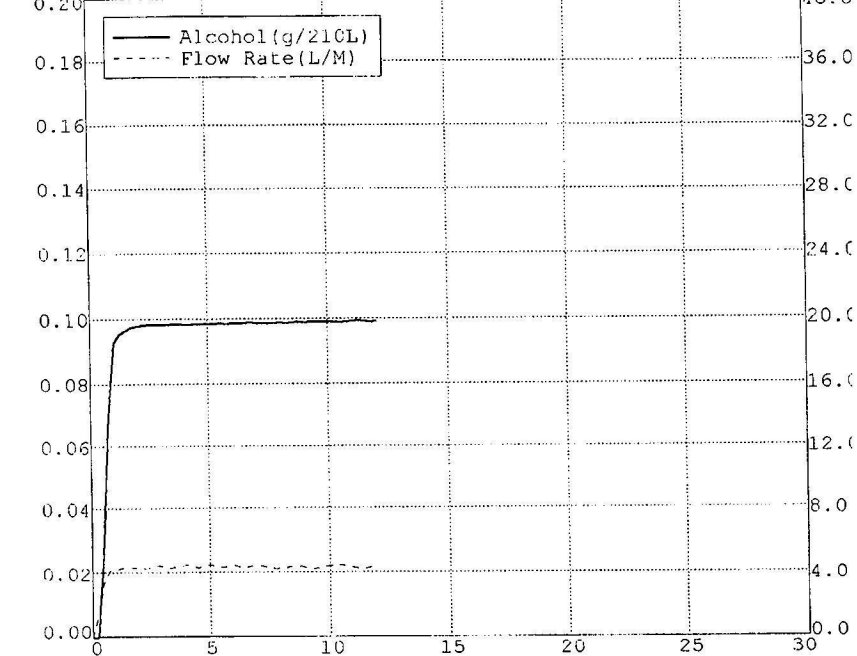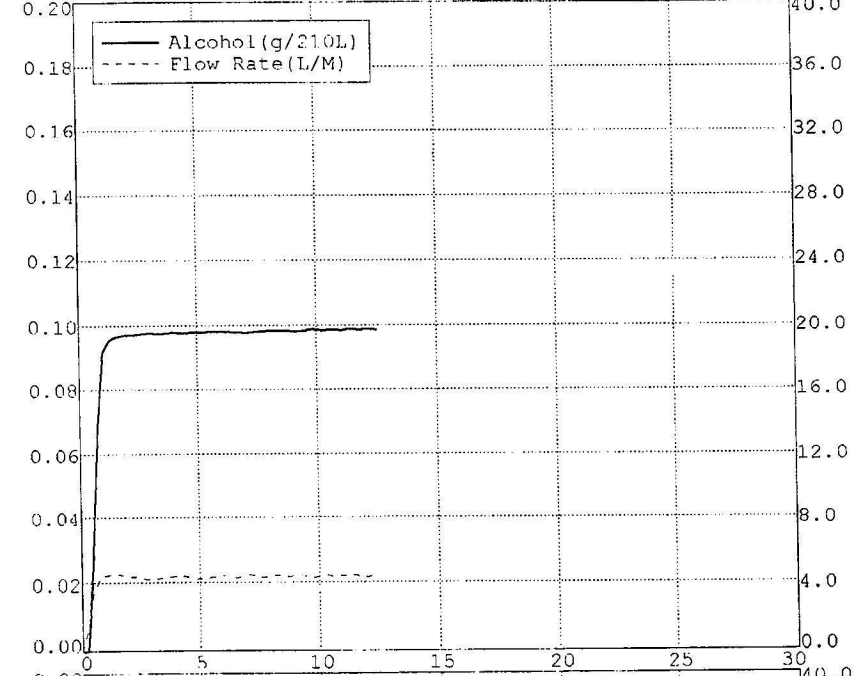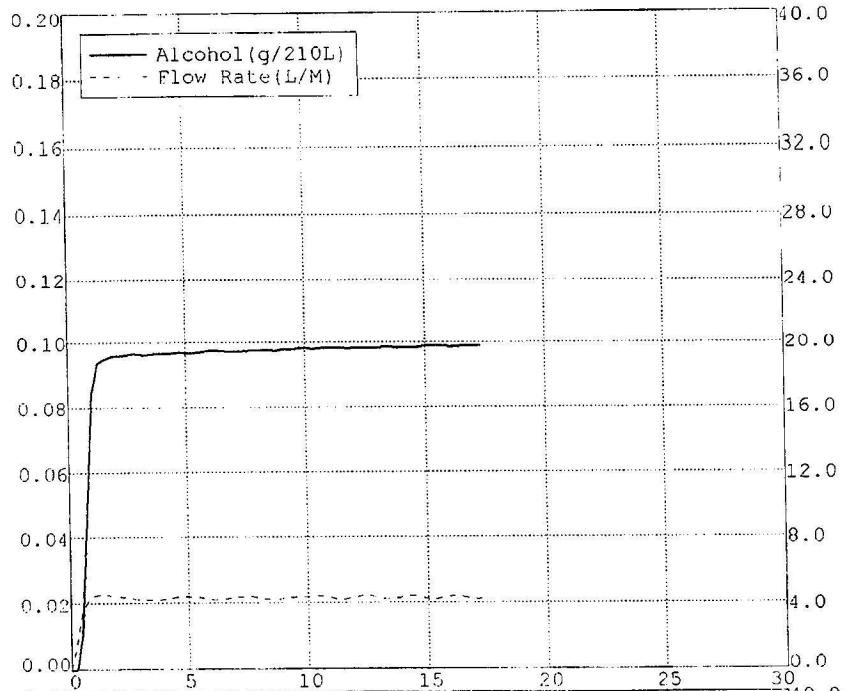

0614