

SOLUTION CHANGE

SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 03/01/2022

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:27
INTERNAL STANDARD	VERIFIED	08:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:28
BLANK TEST	0.00	08:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:29
BLANK TEST	0.00	08:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:30
BLANK TEST	0.00	08:31

ALCOHOL REFERENCE SOLUTION
FOR SIMULATOR

11
BOT. NO.


5/17/22
EXP. DATE

21440
LOT NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH
A PROPERLY OPERATING BREATH SIMULATOR AND
BREATH ALCOHOL ANALYZER, THE SOLUTION WILL
PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTHI LABORATORIES, INC.
HARRISBURG, PENNSYLVANIA 17111

Rev. 1/06

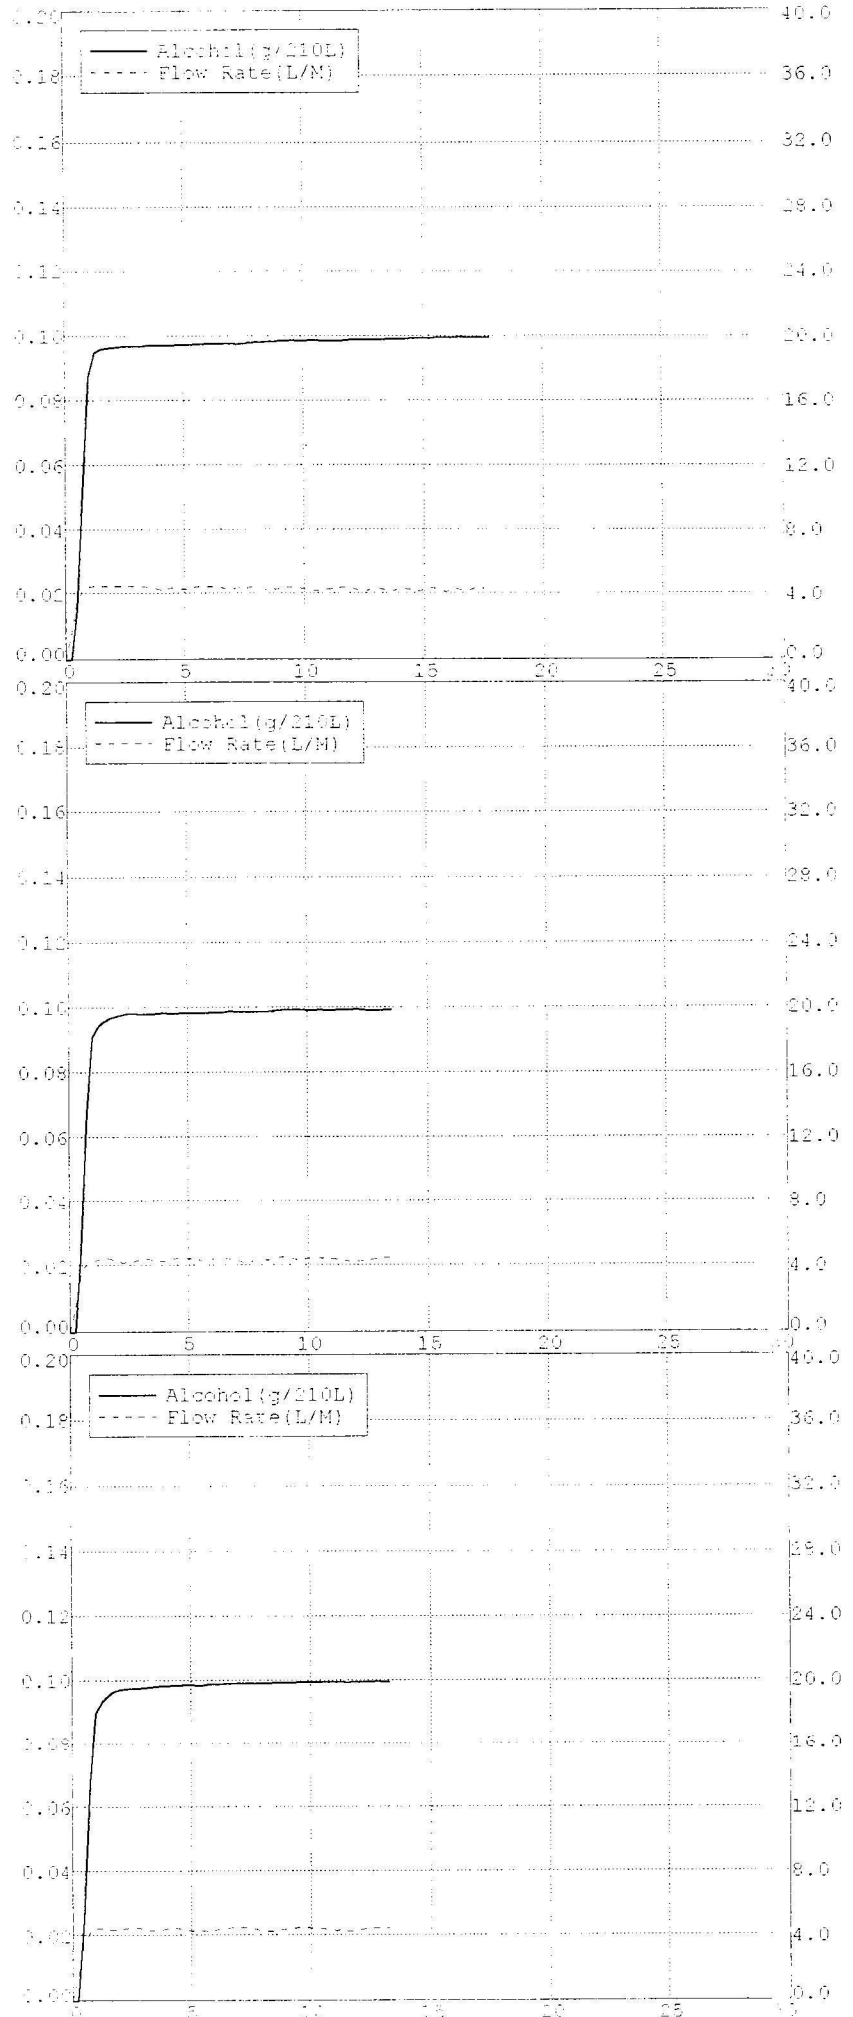

@ 614