

SUPERVISOR TEST




 SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 03/22/2022

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:15
INTERNAL STANDARD	VERIFIED	16:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:15
BLANK TEST	0.00	16:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:17
BLANK TEST	0.00	16:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:18
BLANK TEST	0.00	16:19

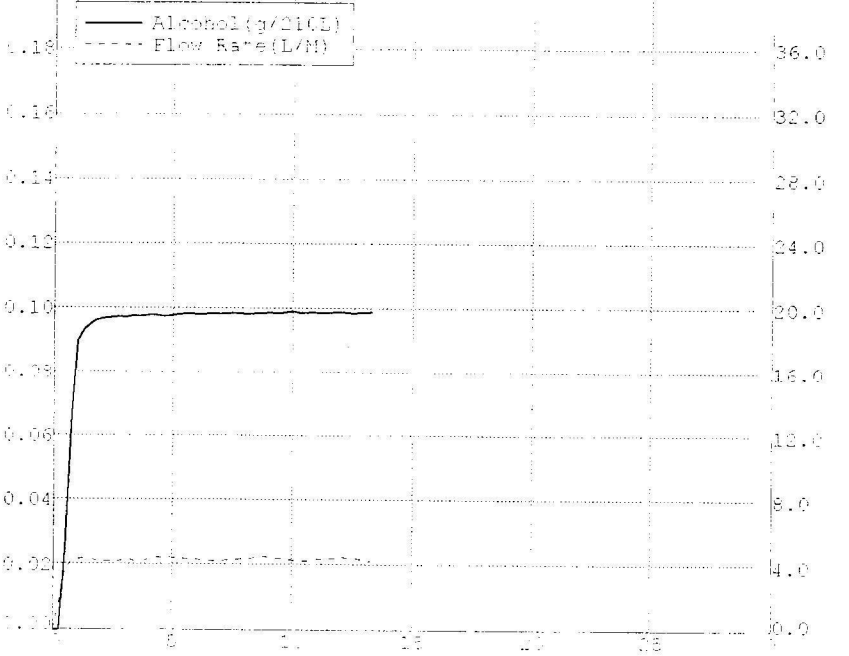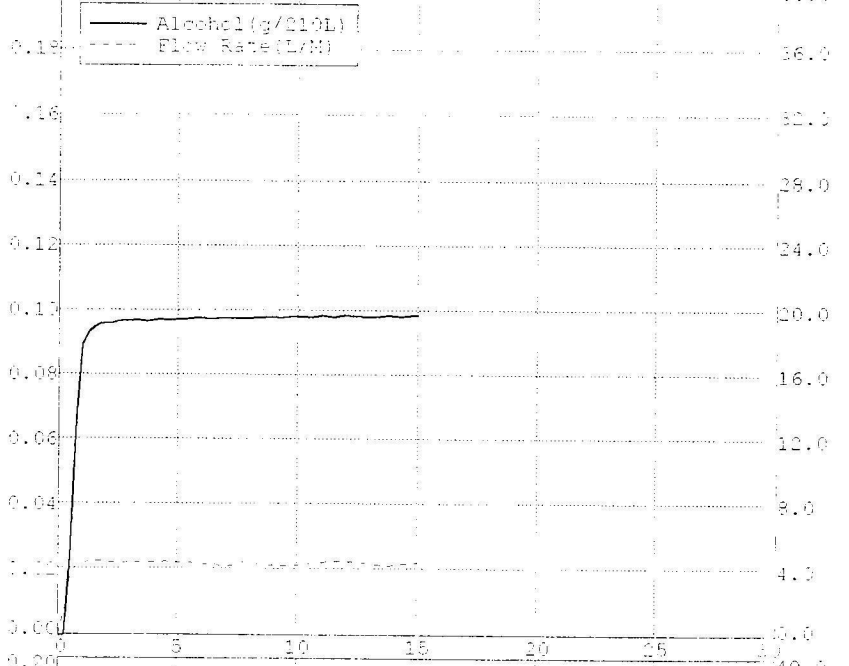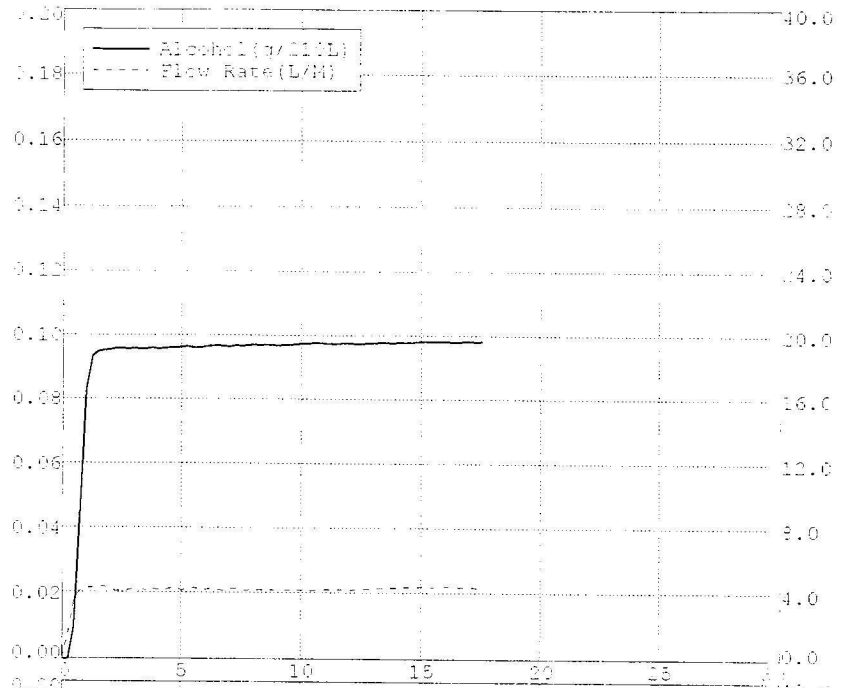

614