

SUPERVISOR TEST




 SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 03/30/2022

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:28
INTERNAL STANDARD	VERIFIED	08:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:29
BLANK TEST	0.00	08:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:30
BLANK TEST	0.00	08:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:31
BLANK TEST	0.00	08:32

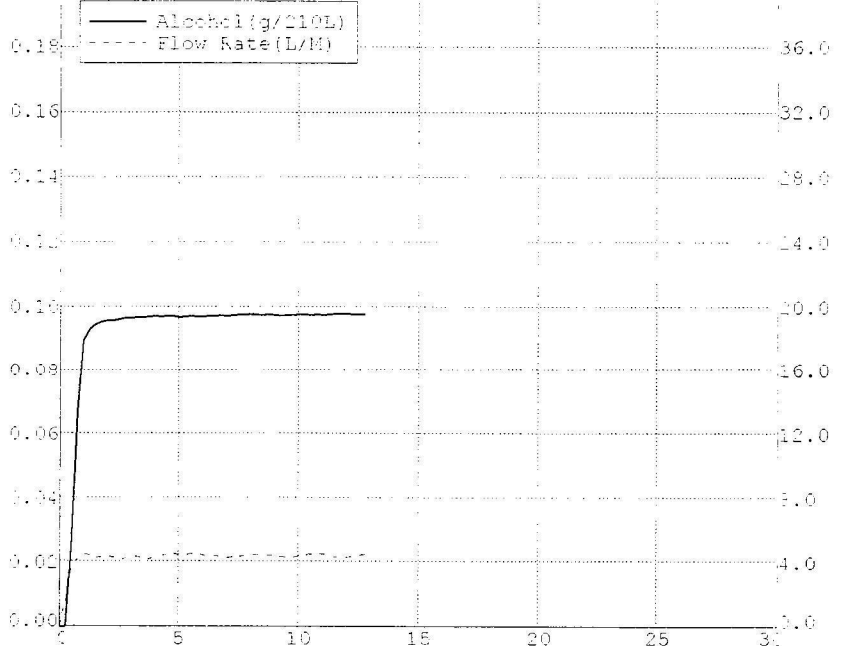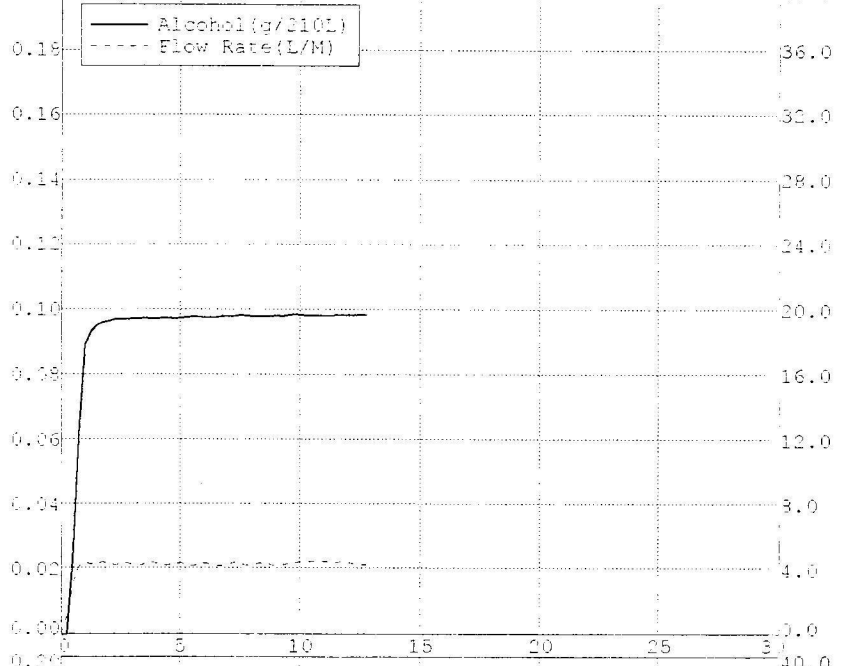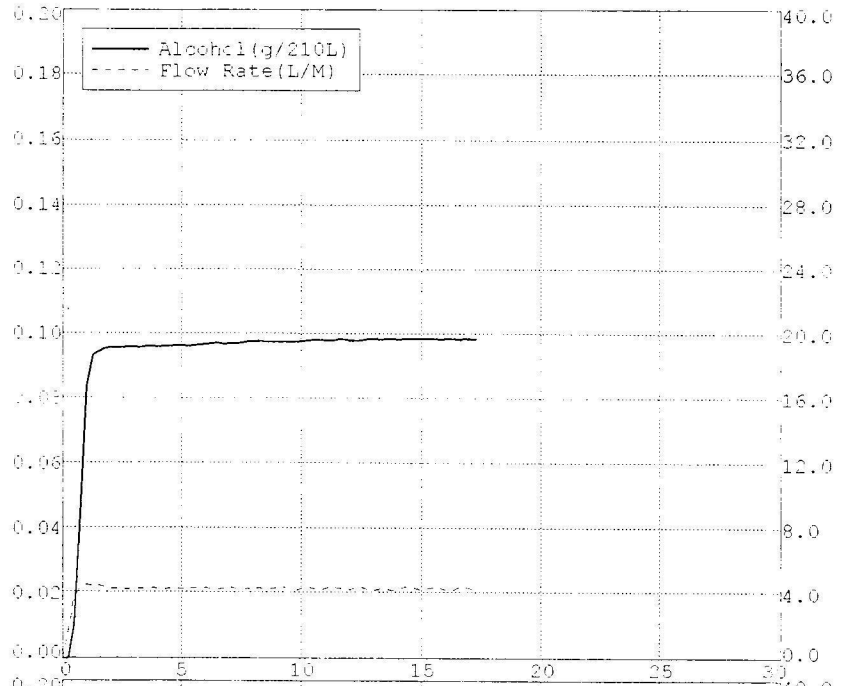

0614