

SOLUTION CHANGE

 SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 04/01/2022

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:21
INTERNAL STANDARD	VERIFIED	08:21
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	08:21
BLANK TEST	0.00	08:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:23
BLANK TEST	0.00	08:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:24
BLANK TEST	0.00	08:25

ALCOHOL REFERENCE SOLUTION
 FOR SIMULATOR

22030
 LOT NO.




7/24/22
 EXP. DATE

1097
 BOT. NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH
 A PROPERLY OPERATING BREATH SIMULATOR AND
 BREATH ALCOHOL ANALYZER, THE SOLUTION WILL
 PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.
 HARRISBURG, PENNSYLVANIA 17111

Rev. 1/06

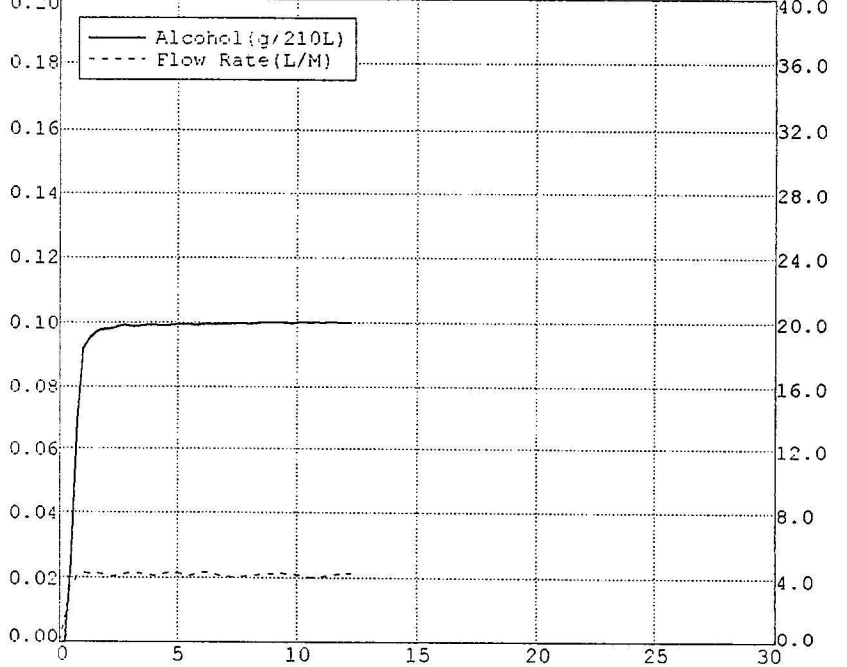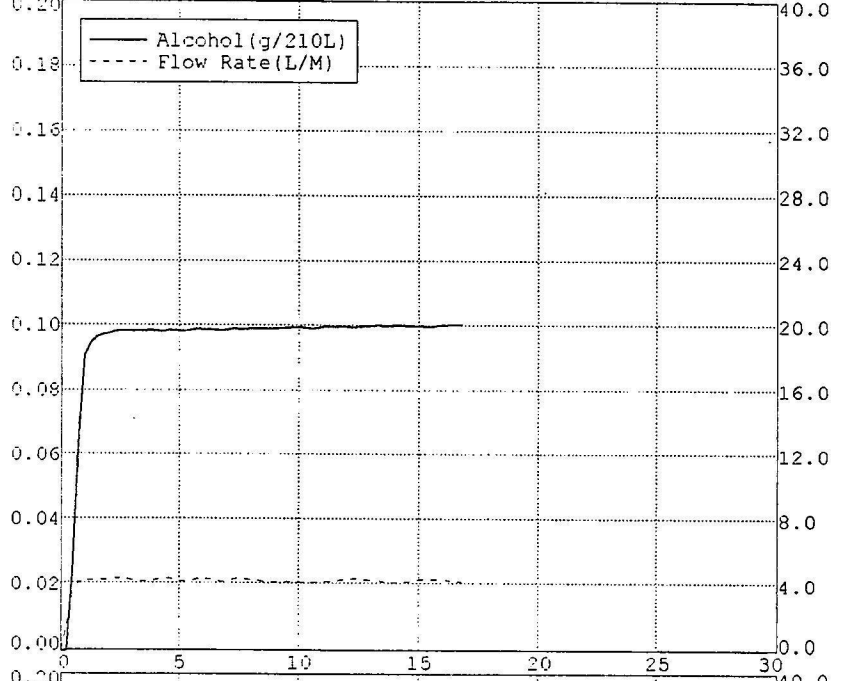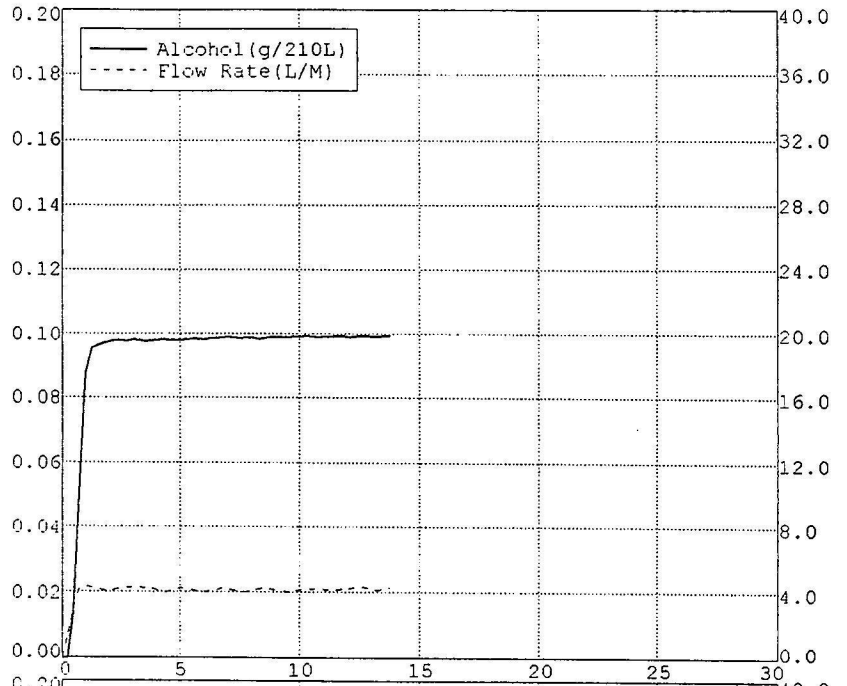

614