

SUPERVISOR TEST




-----  
SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106  
-----

Date: 04/06/2022

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:24
INTERNAL STANDARD	VERIFIED	16:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:25
BLANK TEST	0.00	16:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:26
BLANK TEST	0.00	16:27
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	16:27
BLANK TEST	0.00	16:28

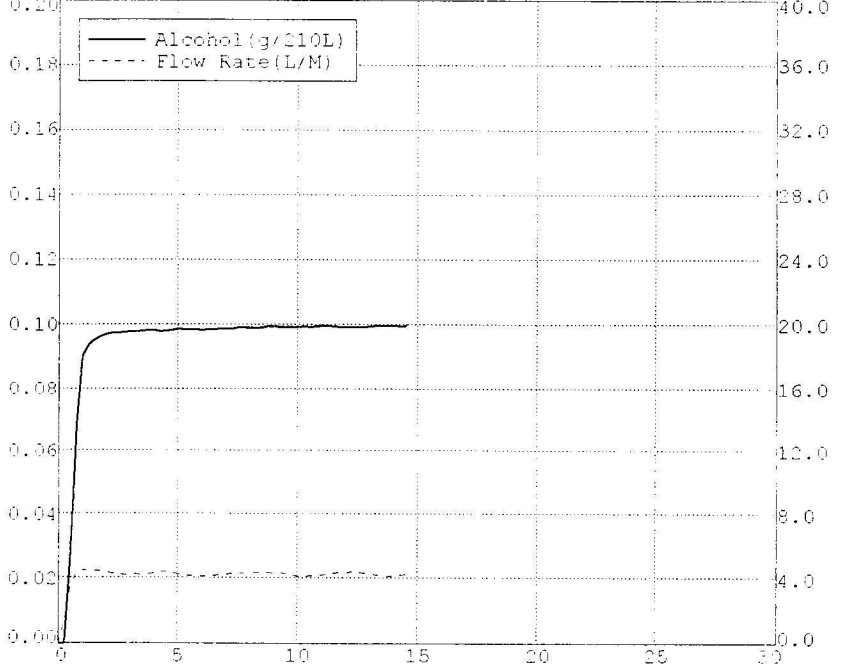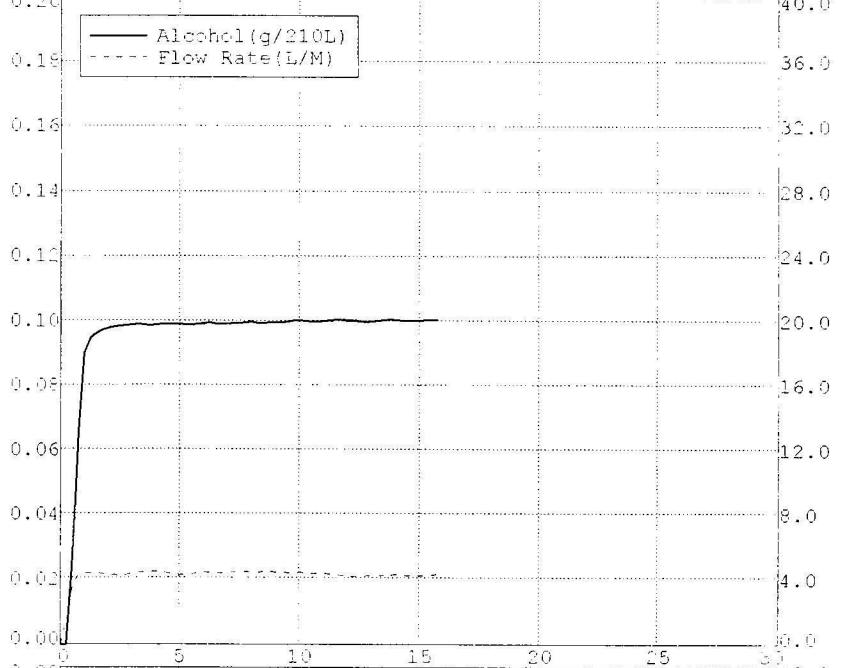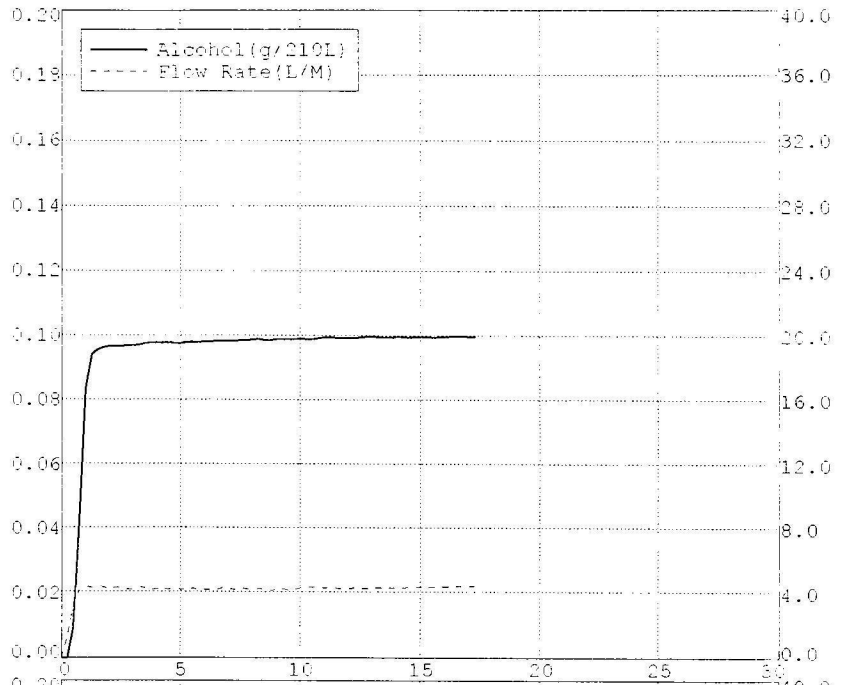

*Handwritten signature and number 614*