

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 04/14/2022

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:37
INTERNAL STANDARD	VERIFIED	08:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:38
BLANK TEST	0.00	08:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:39
BLANK TEST	0.00	08:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:41
BLANK TEST	0.00	08:42

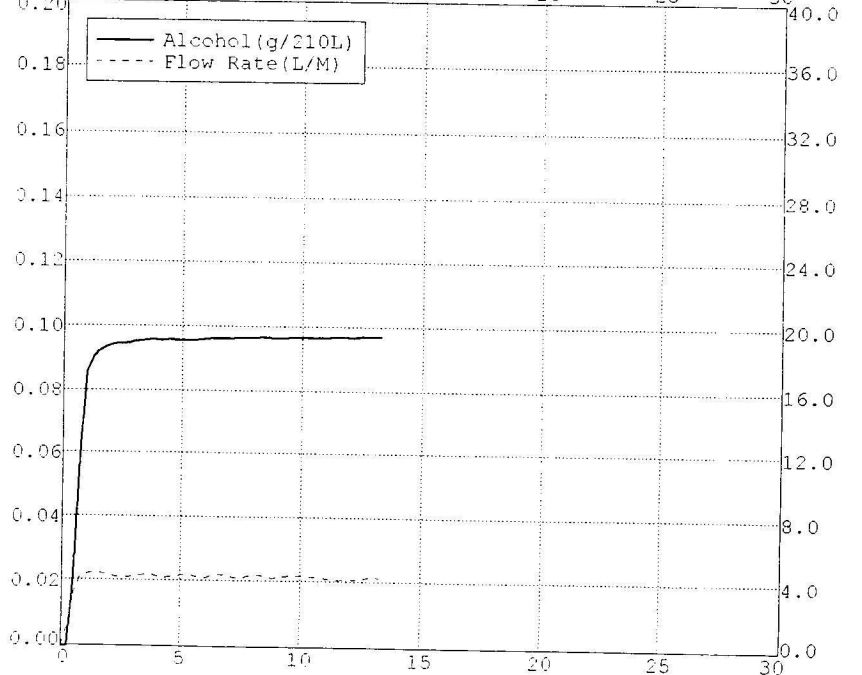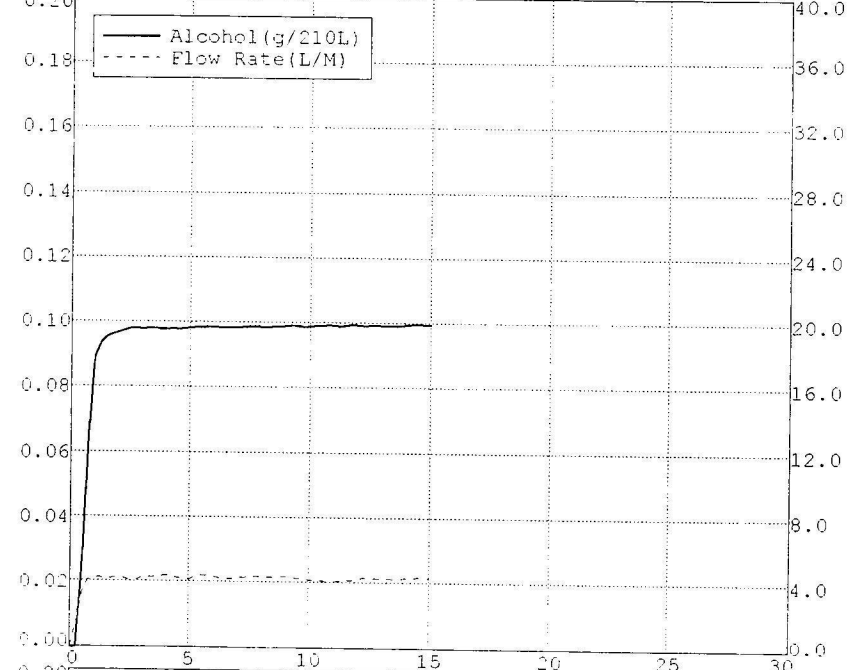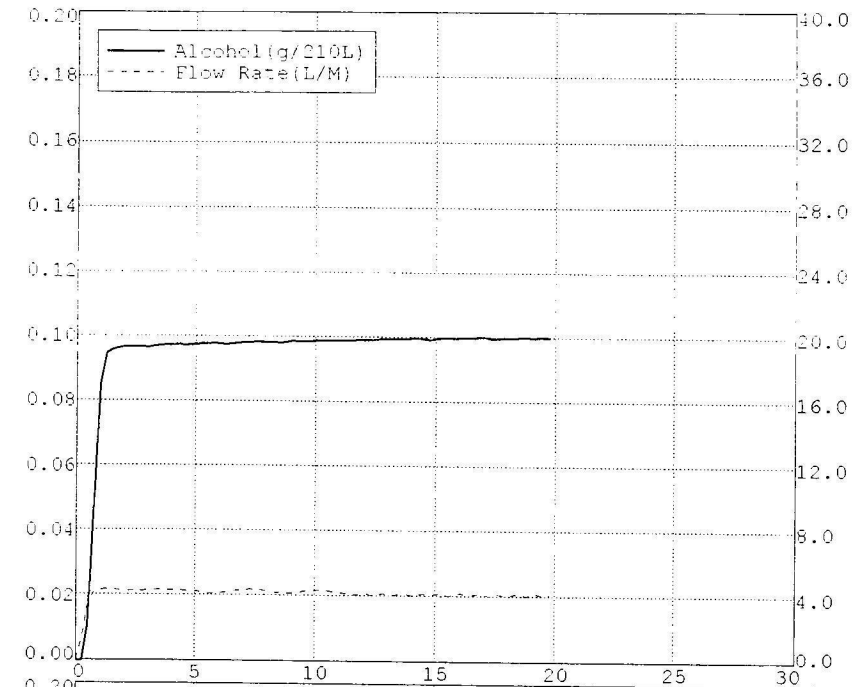

2014