

SOLUTION CHANGE




 SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 05/02/2022

OPERATOR NAME:
 ANDREW S COLE-HATCHARD
 Permit #: 47565
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:06
INTERNAL STANDARD	VERIFIED	09:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:06
BLANK TEST	0.00	09:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:08
BLANK TEST	0.00	09:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:09
BLANK TEST	0.00	09:10

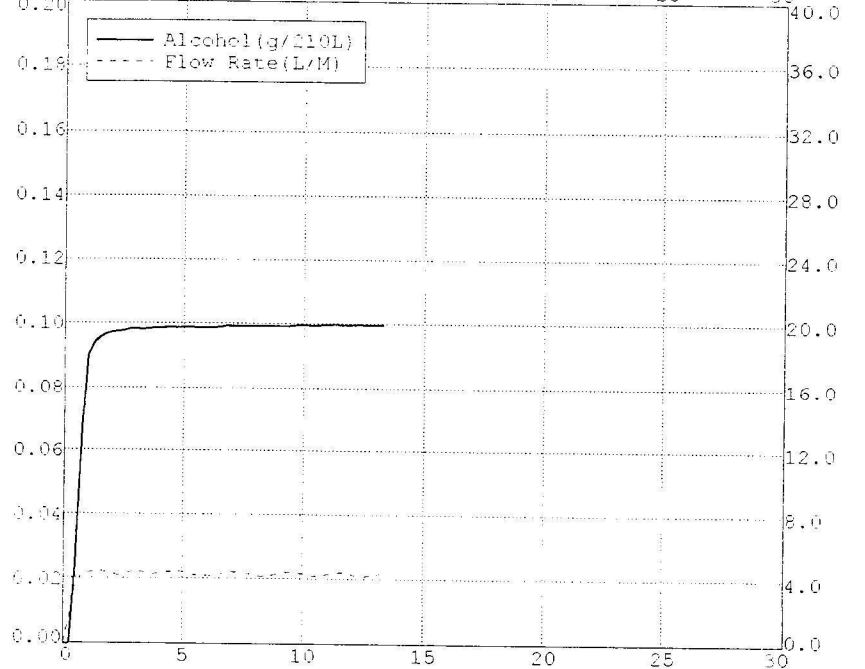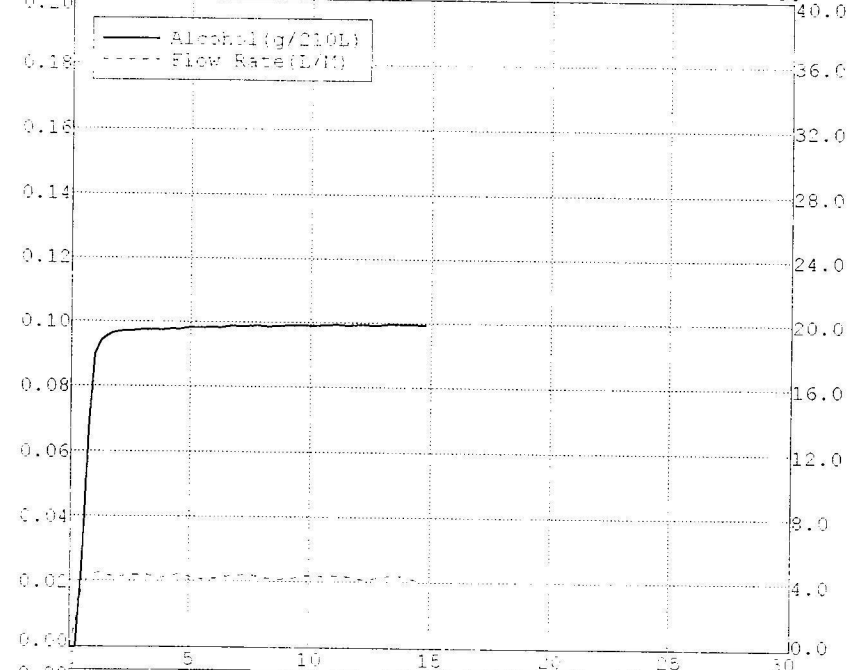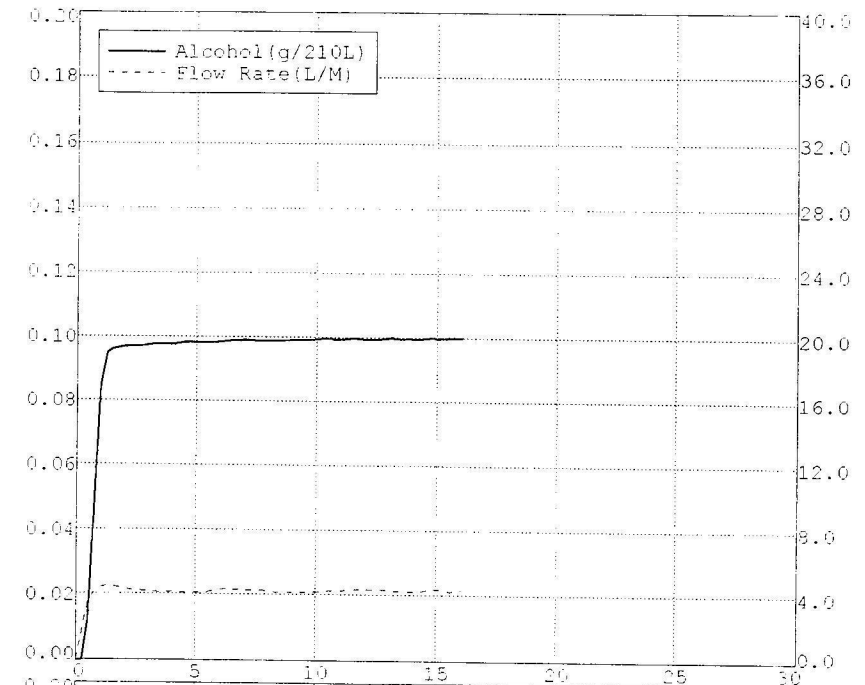

② bus

