

SUPERVISOR TEST




 SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 05/09/2022

OPERATOR NAME:
 ANDREW S COLE-HATCHARD
 Permit #: 47565
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:29
INTERNAL STANDARD	VERIFIED	16:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:29
BLANK TEST	0.00	16:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:31
BLANK TEST	0.00	16:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:32
BLANK TEST	0.00	16:33

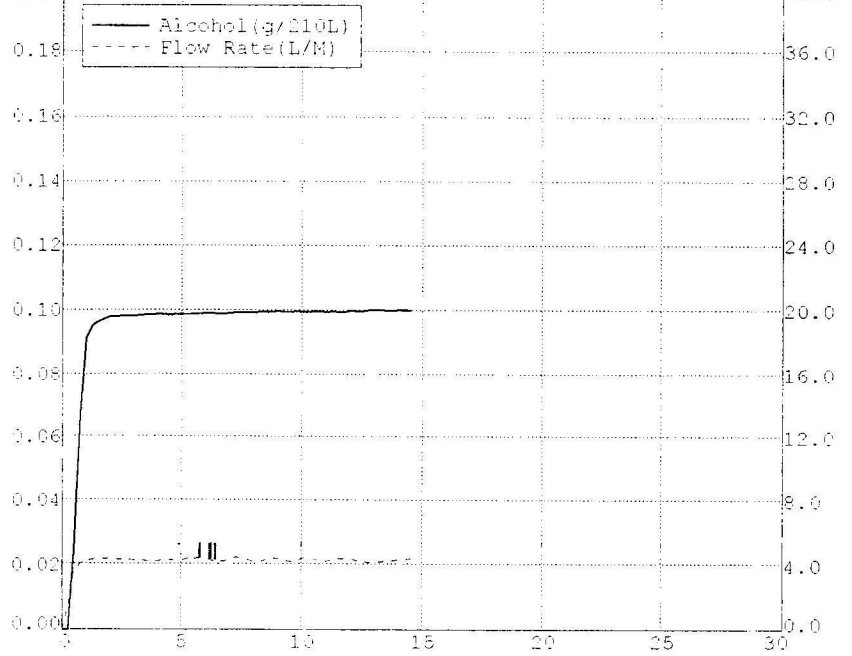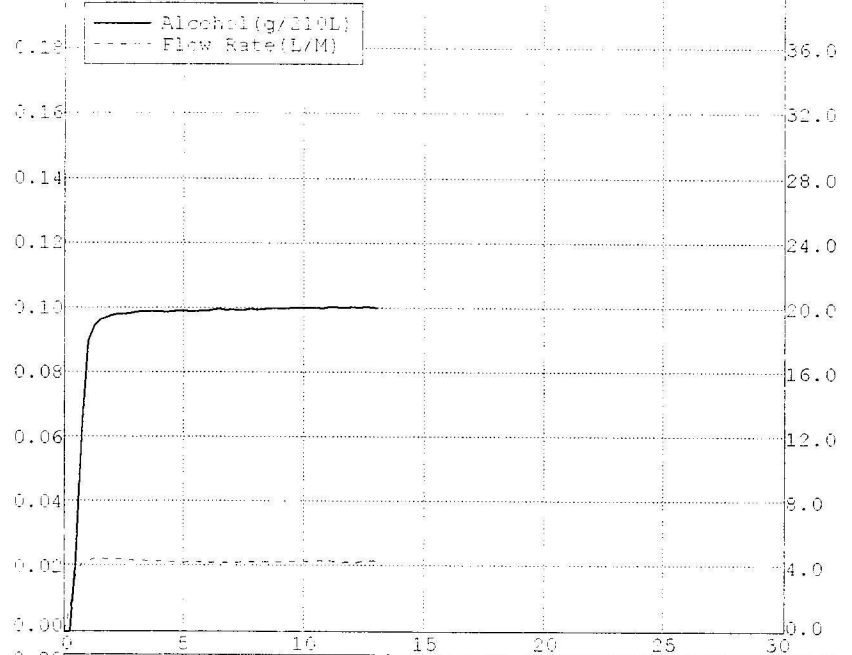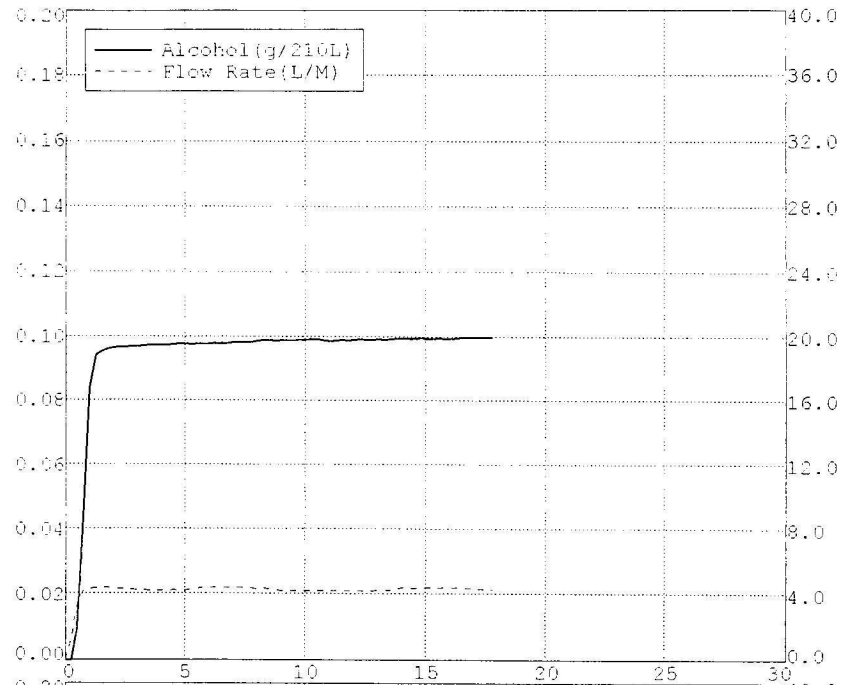

AC