

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 05/16/2022

OPERATOR NAME:
ANDREW S COLE-HATCHARD
Permit #: 47565
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:51
INTERNAL STANDARD	VERIFIED	07:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:51
BLANK TEST	0.00	07:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:53
BLANK TEST	0.00	07:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:54
BLANK TEST	0.00	07:55

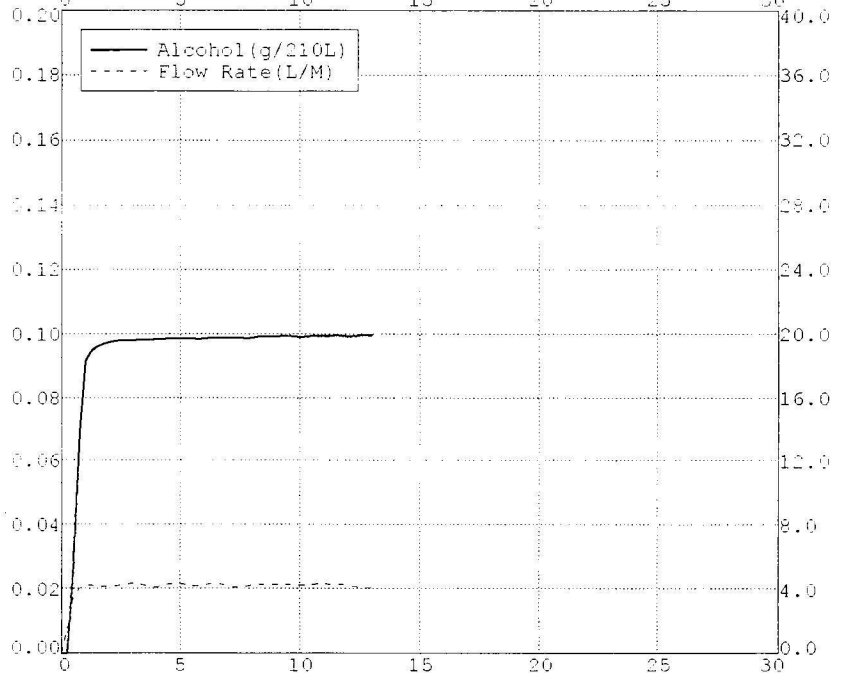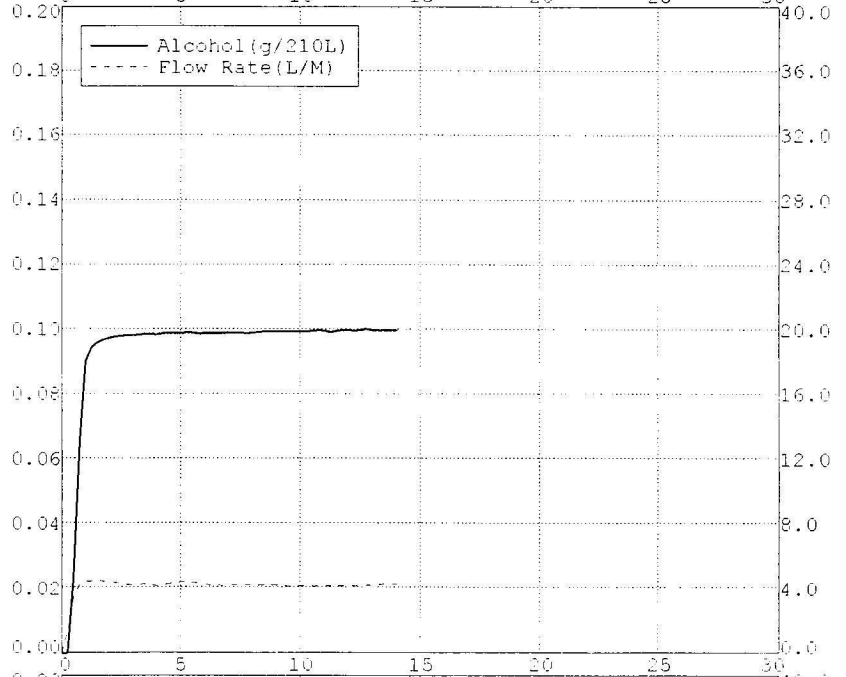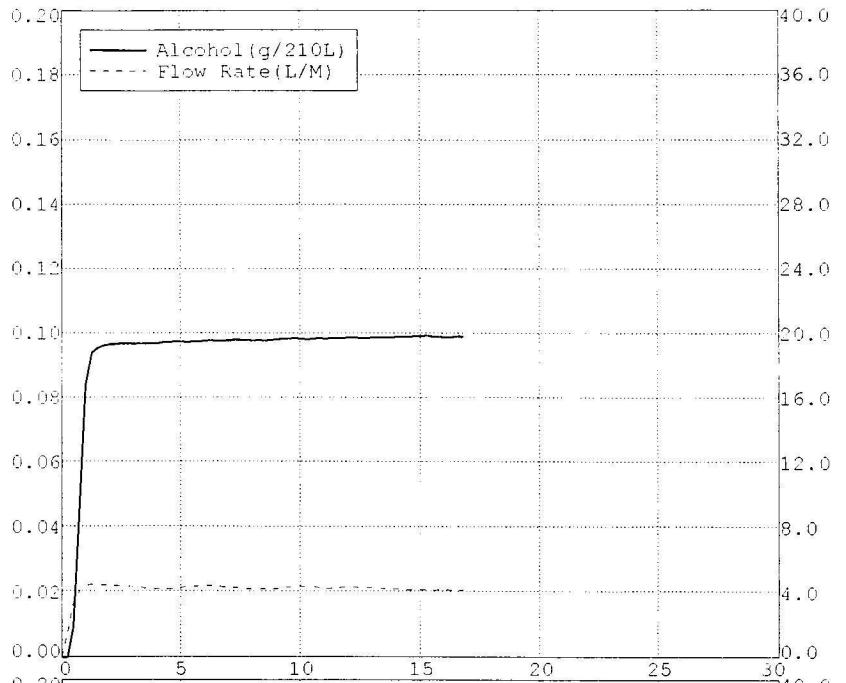

Handwritten signature/initials