

SUPERVISOR TEST




SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 05/30/2022

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:40
INTERNAL STANDARD	VERIFIED	15:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:41
BLANK TEST	0.00	15:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:42
BLANK TEST	0.00	15:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:43
BLANK TEST	0.00	15:44

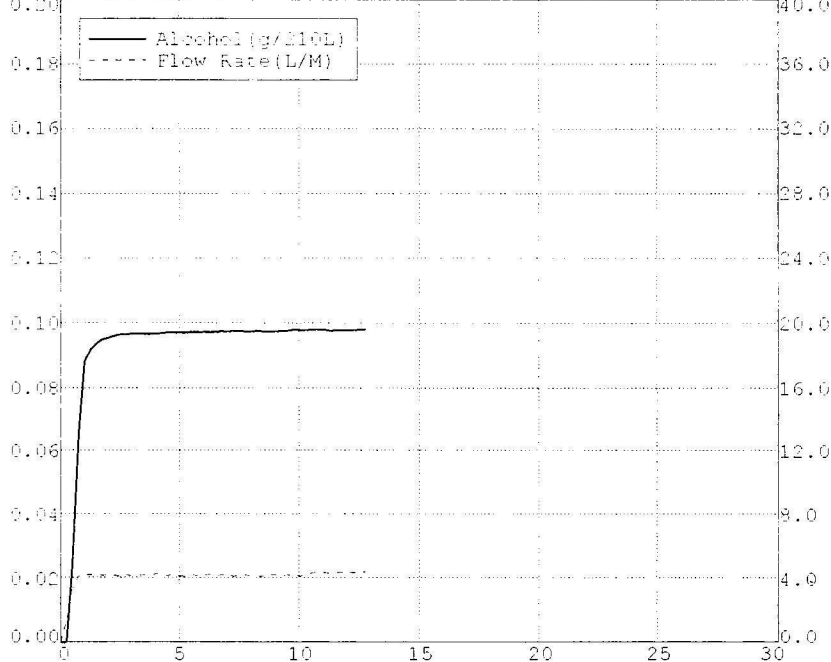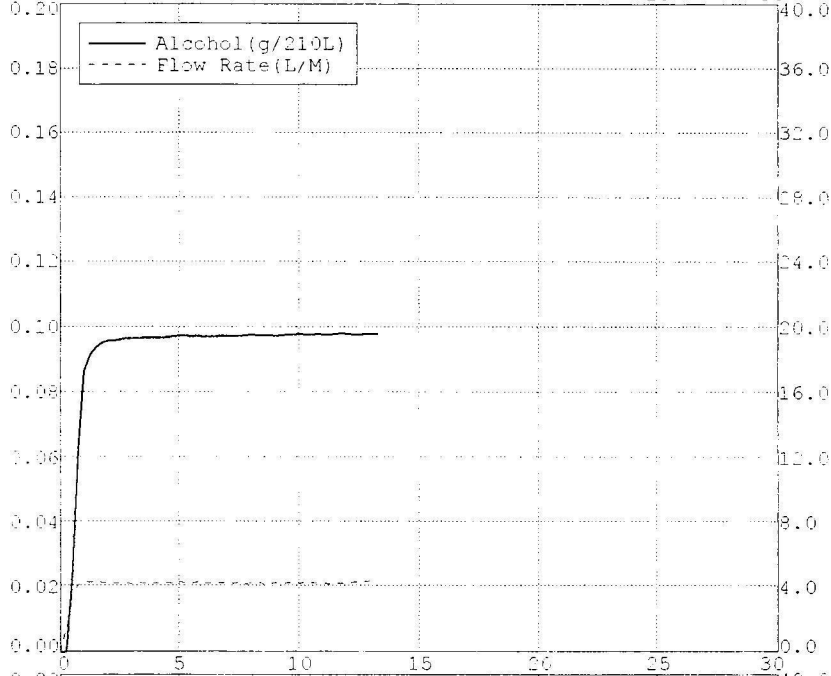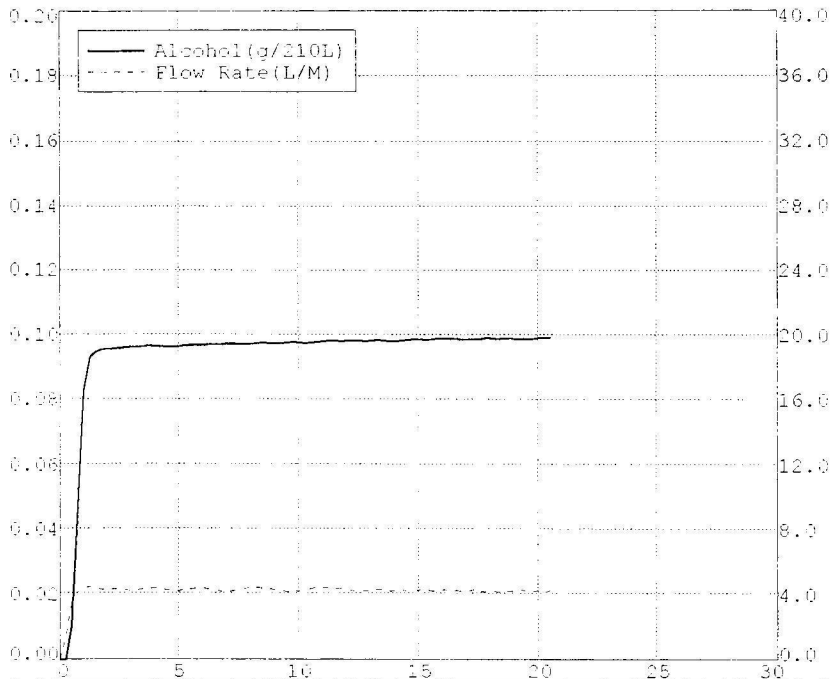

614