

SOLUTION CHANGE




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 06/01/2022

OPERATOR NAME:
ANDREW S COLE-HATCHARD
Permit #: 47565
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:10
INTERNAL STANDARD	VERIFIED	11:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:11
BLANK TEST	0.00	11:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:12
BLANK TEST	0.00	11:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:13
BLANK TEST	0.00	11:14

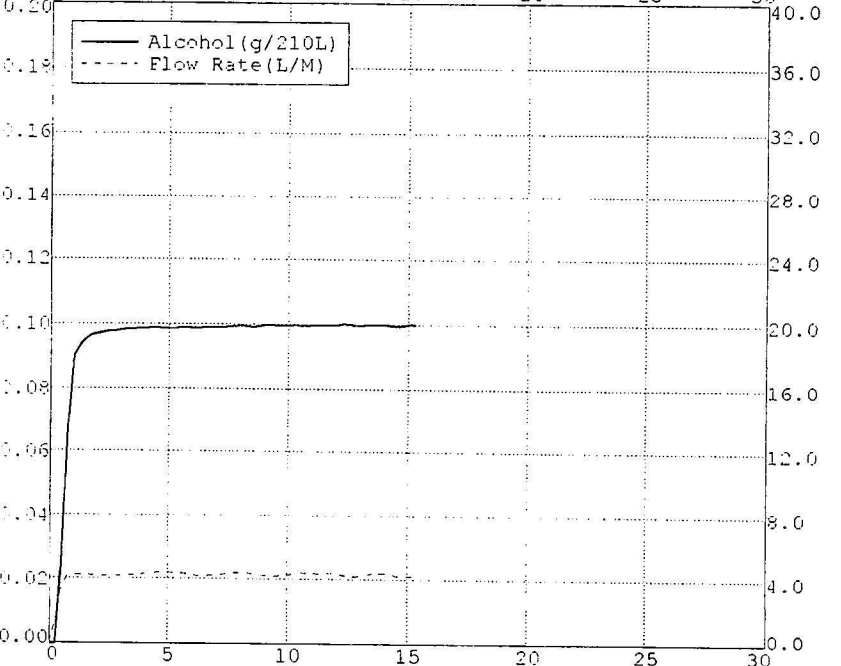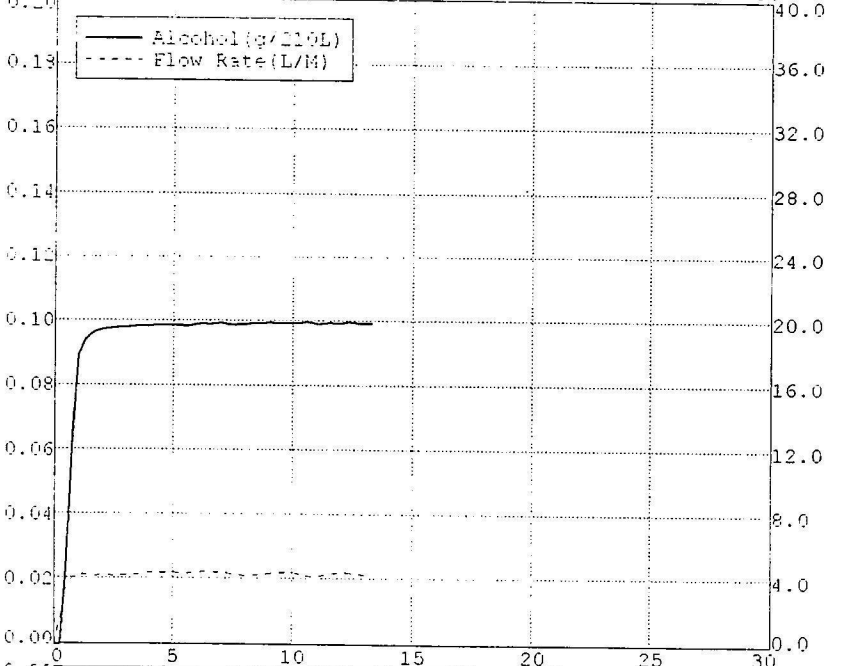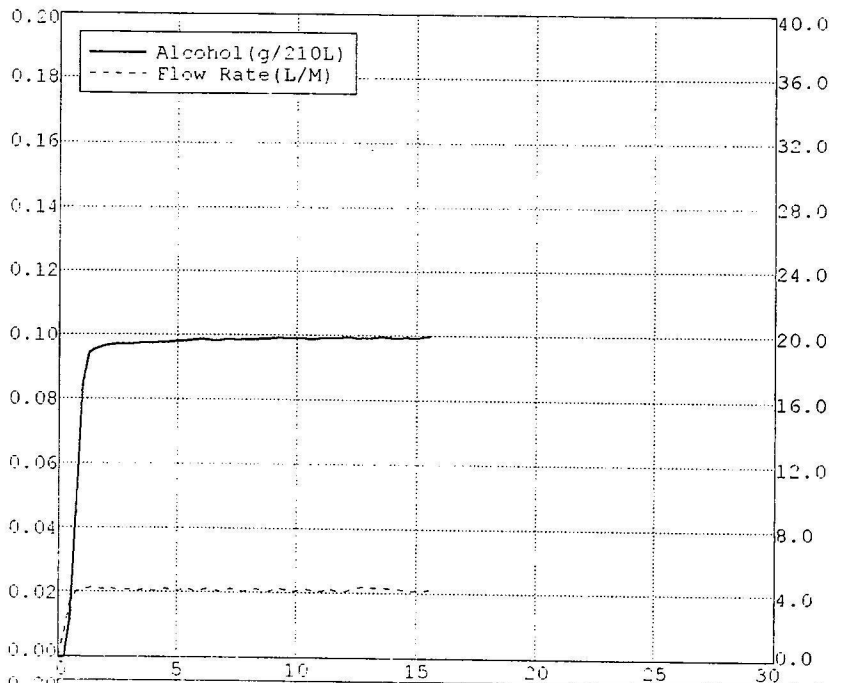

ALCOHOL REFERENCE SOLUTION
FOR SIMULATOR

22100
LOT NO.

9/28/22
EXP. DATE

1437
BOT. NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH
A PROPERLY OPERATING BREATH SIMULATOR AND
BREATH ALCOHOL ANALYZER, THE SOLUTION WILL
PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.
HARRISBURG, PENNSYLVANIA 17111

Rev. 1/06

PC L- ~~111~~ 645

