

SUPERVISOR TEST




 SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 06/13/2022

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:31
INTERNAL STANDARD	VERIFIED	08:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:31
BLANK TEST	0.00	08:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:33
BLANK TEST	0.00	08:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:34
BLANK TEST	0.00	08:35

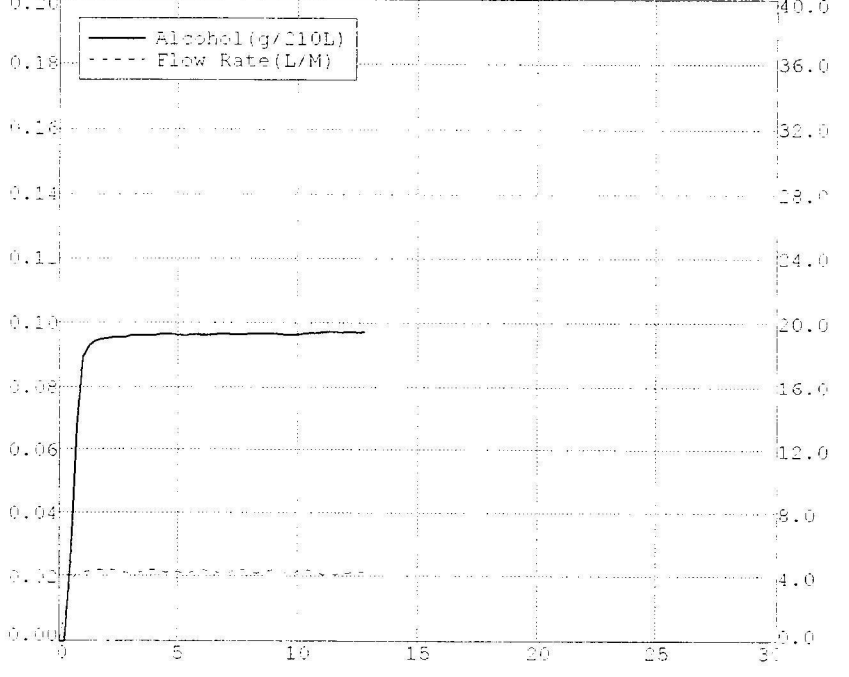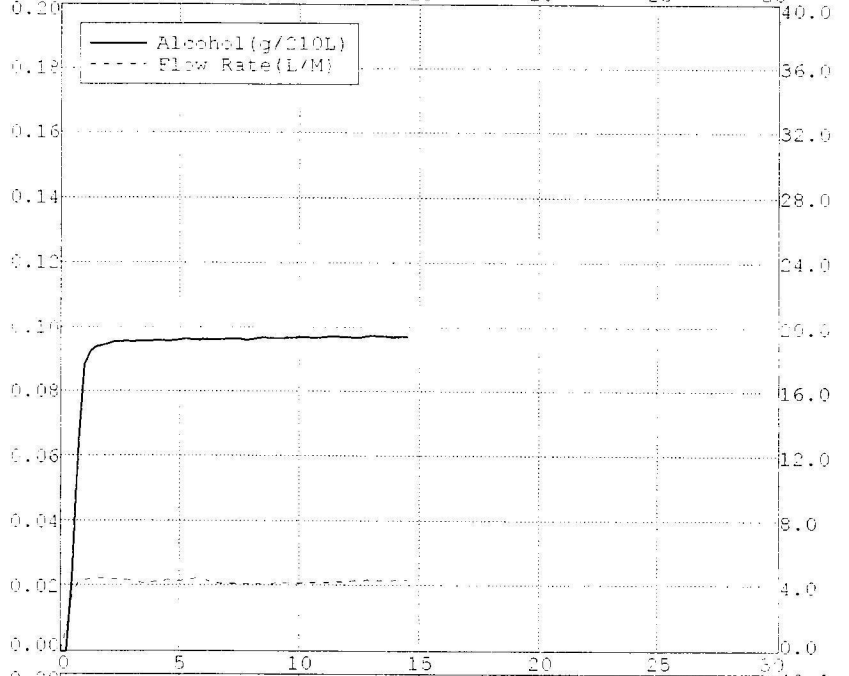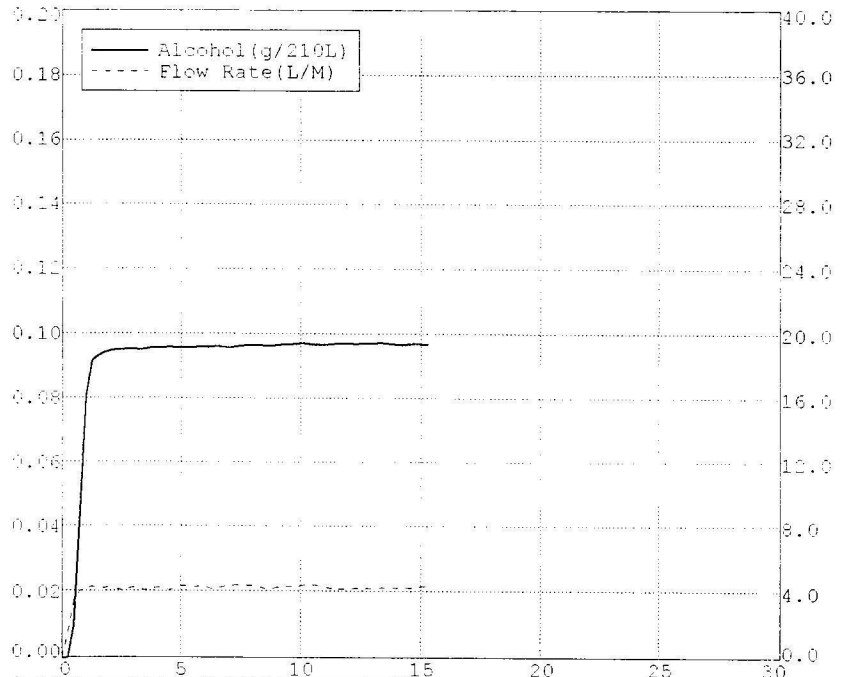

0614