

SUPERVISOR TEST




SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 07/09/2022

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:27
INTERNAL STANDARD	VERIFIED	18:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:28
BLANK TEST	0.00	18:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:29
BLANK TEST	0.00	18:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:31
BLANK TEST	0.00	18:32

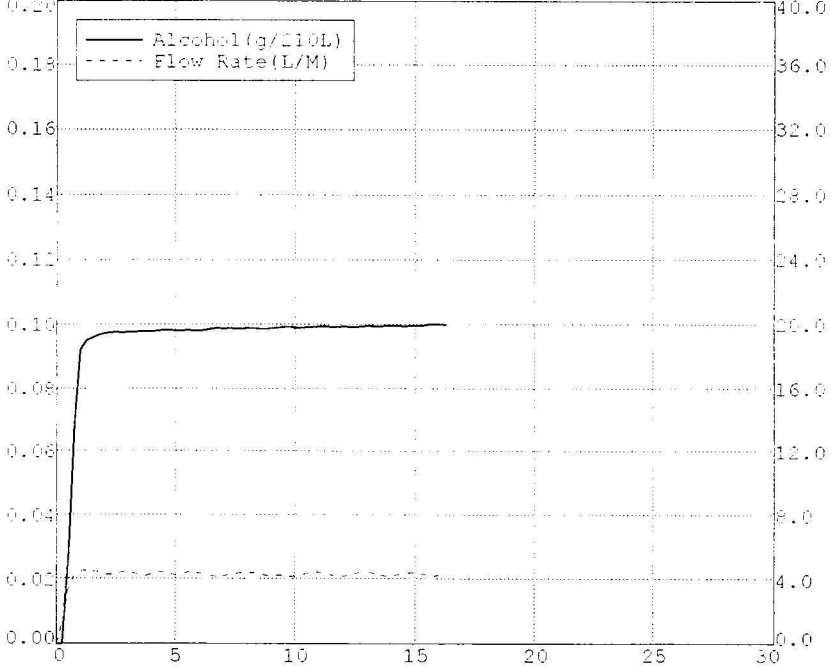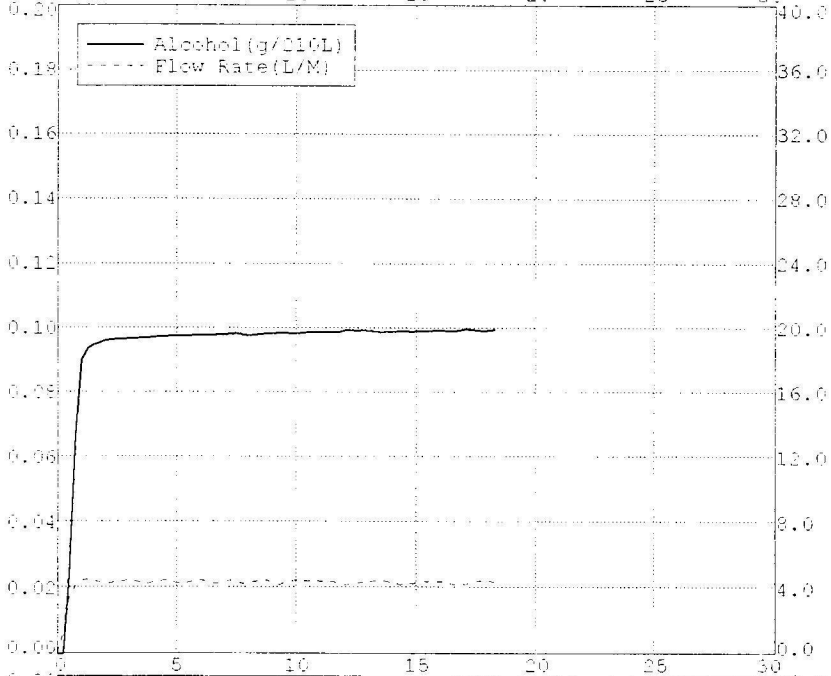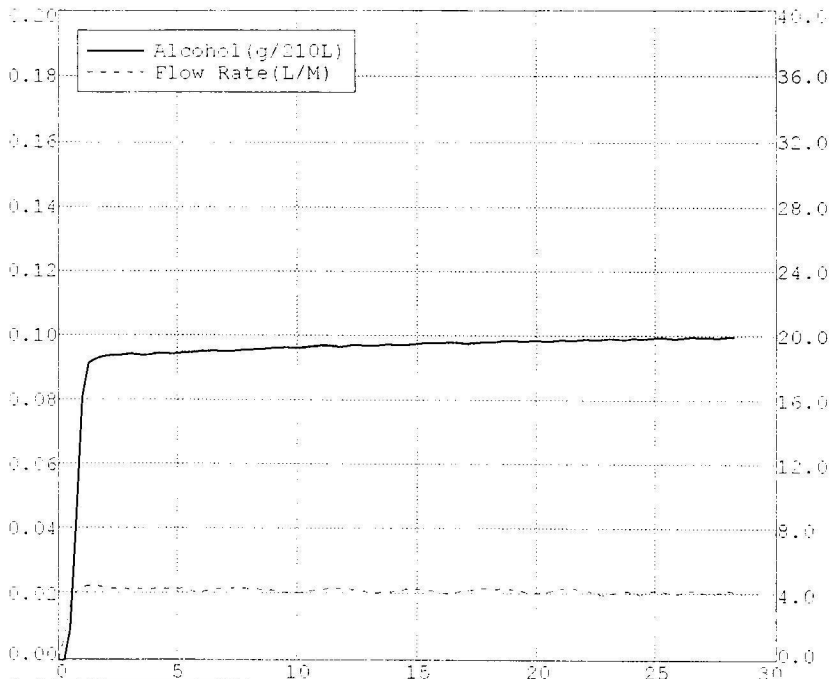

614