

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 07/26/2022

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:28
INTERNAL STANDARD	VERIFIED	00:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:28
BLANK TEST	0.00	00:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:29
BLANK TEST	0.00	00:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:31
BLANK TEST	0.00	00:32

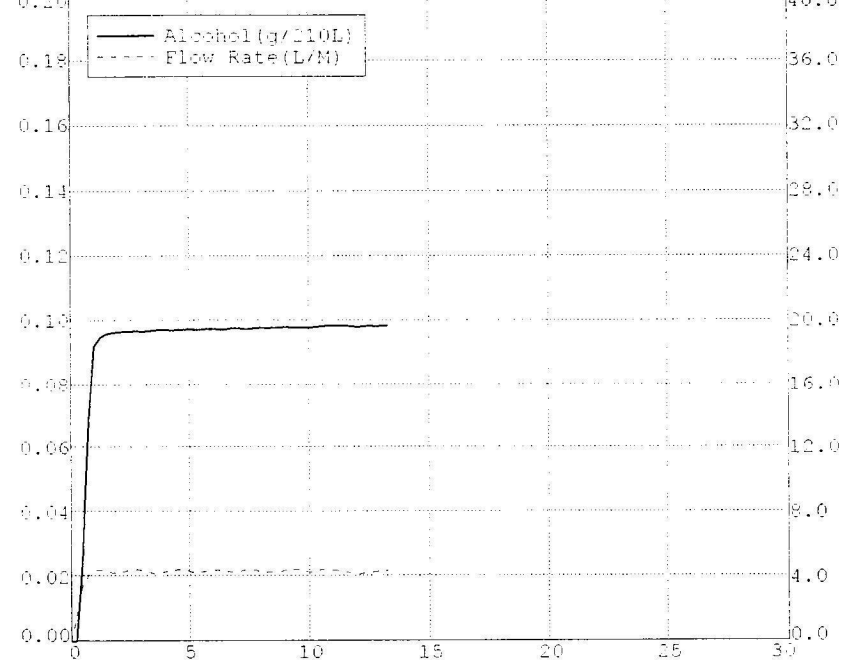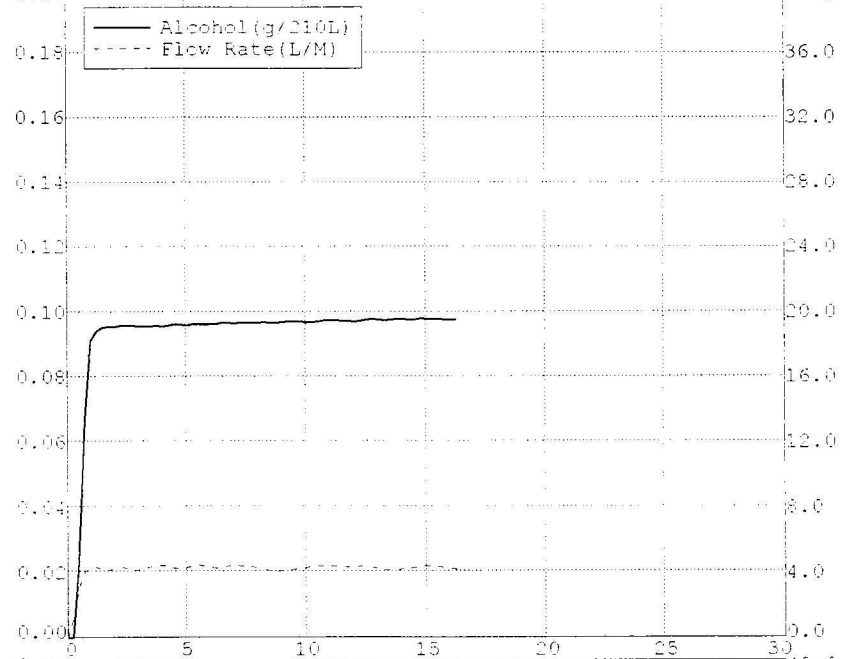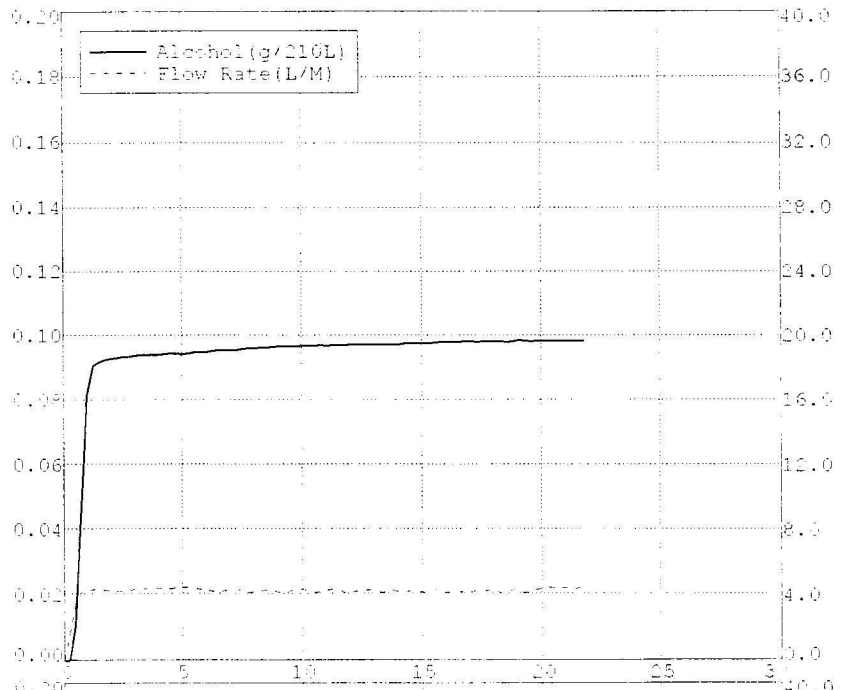

614