

SUPERVISOR TEST




SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 08/08/2022

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:30
INTERNAL STANDARD	VERIFIED	16:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:31
BLANK TEST	0.00	16:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:32
BLANK TEST	0.00	16:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:33
BLANK TEST	0.00	16:34

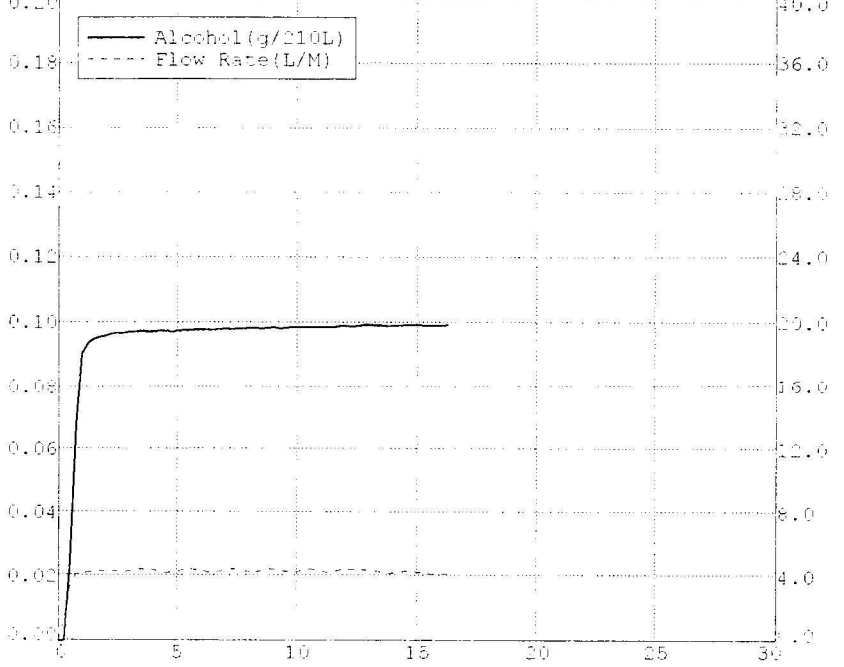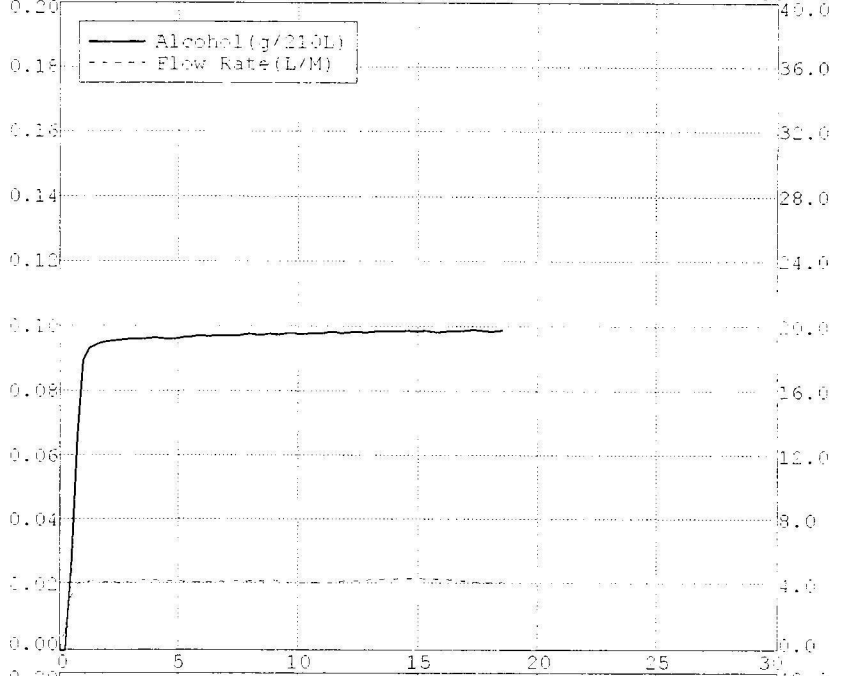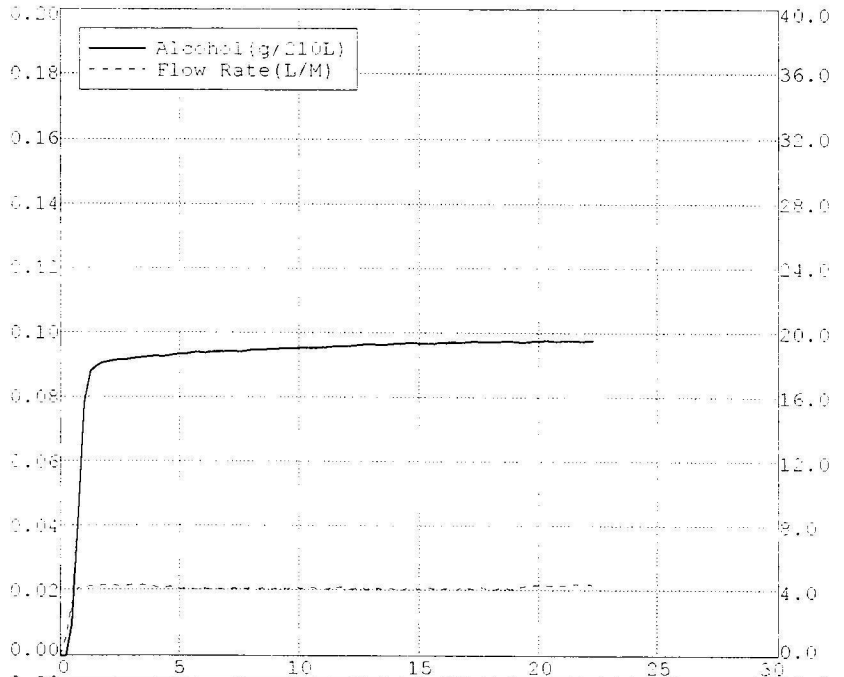

614