

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 08/15/2022

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:00
INTERNAL STANDARD	VERIFIED	10:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:00
BLANK TEST	0.00	10:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:02
BLANK TEST	0.00	10:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:03
BLANK TEST	0.00	10:04

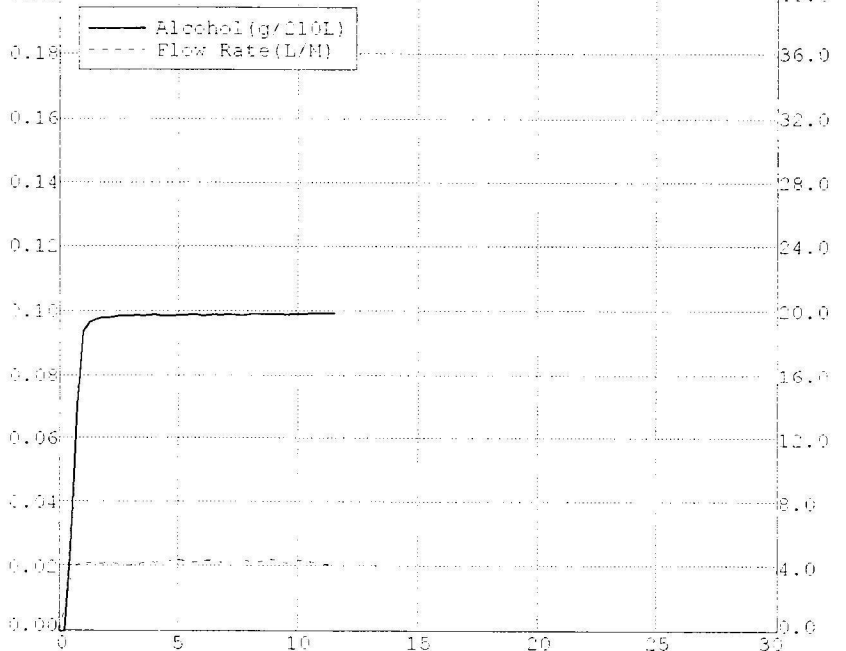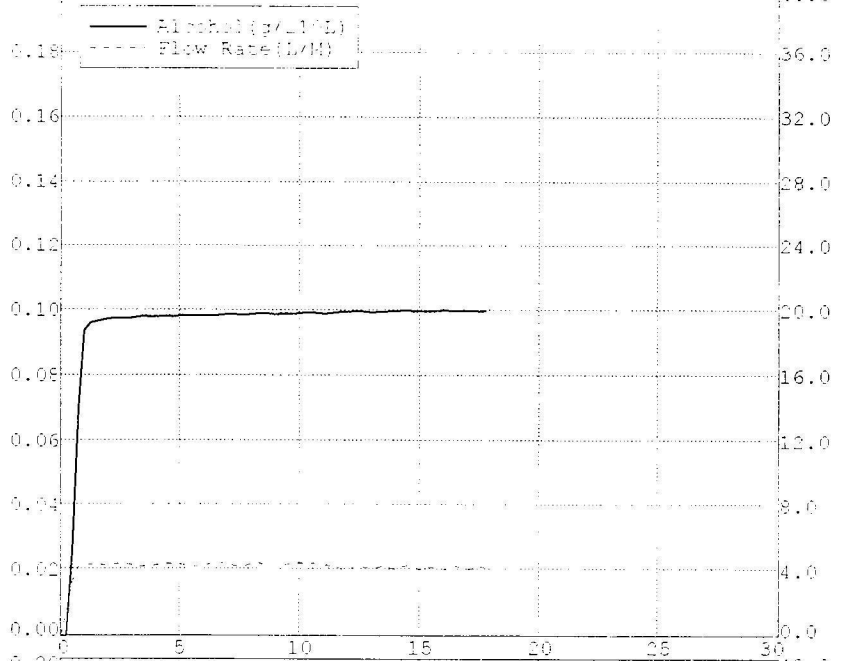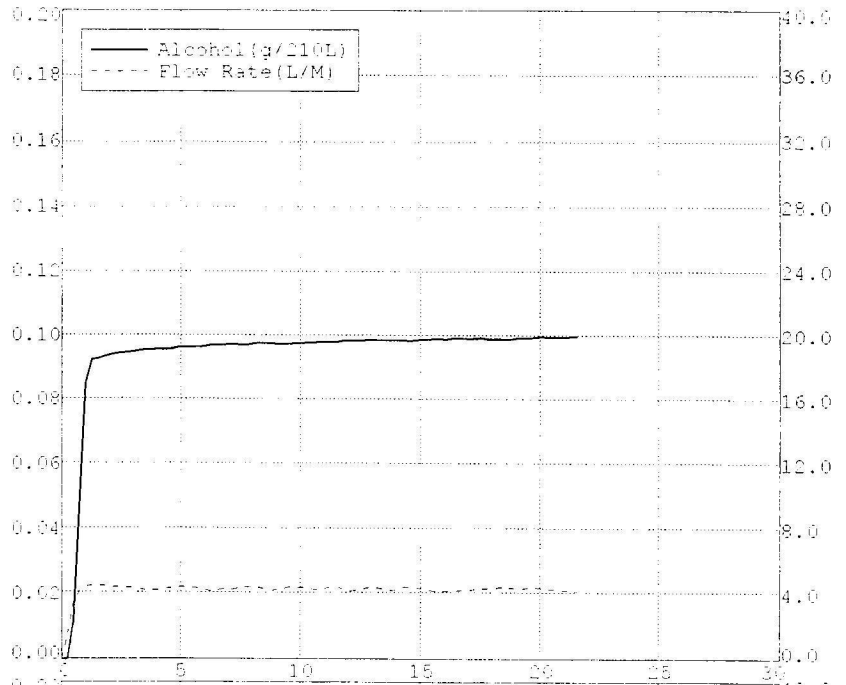

6161