

SUPERVISOR TEST




SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 08/22/2022

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:01
INTERNAL STANDARD	VERIFIED	17:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:02
BLANK TEST	0.00	17:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:03
BLANK TEST	0.00	17:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:04
BLANK TEST	0.00	17:05

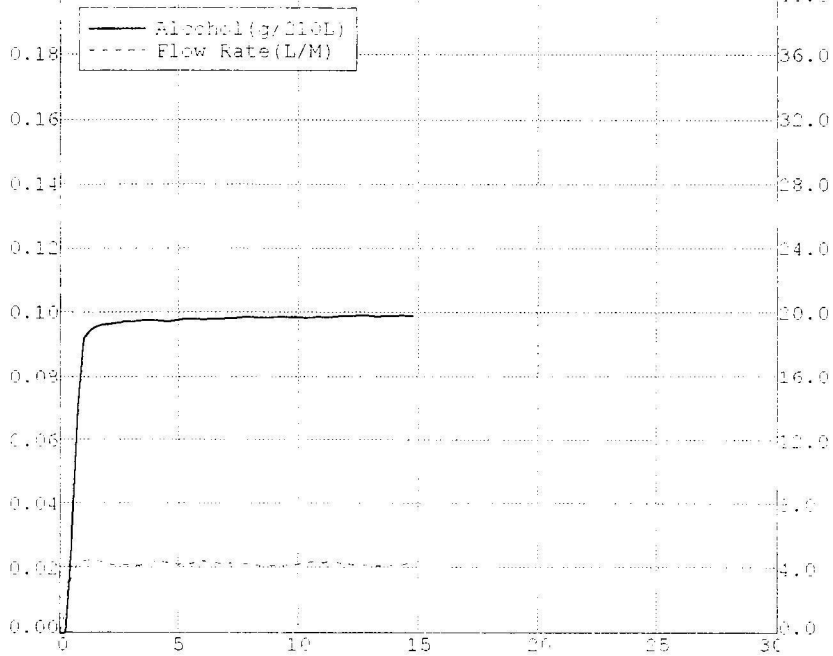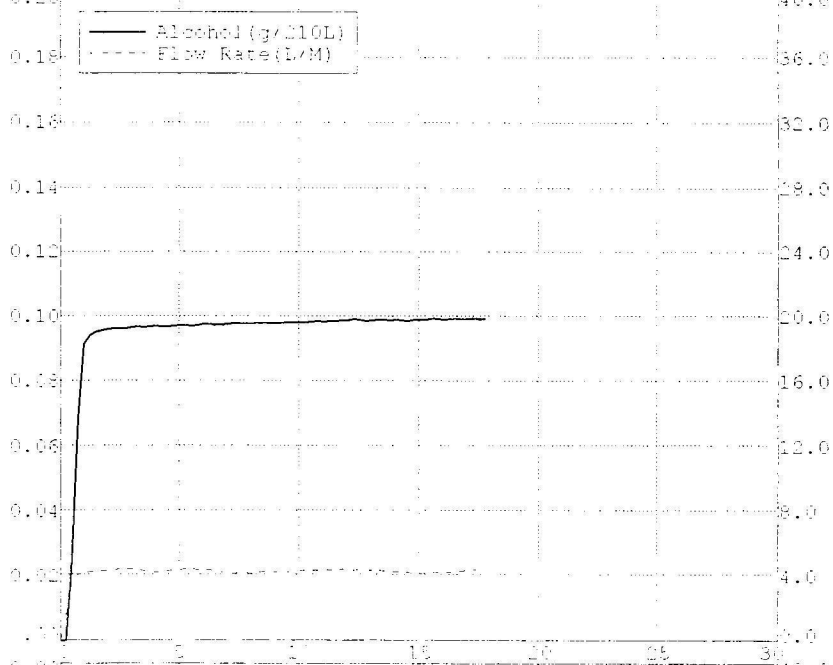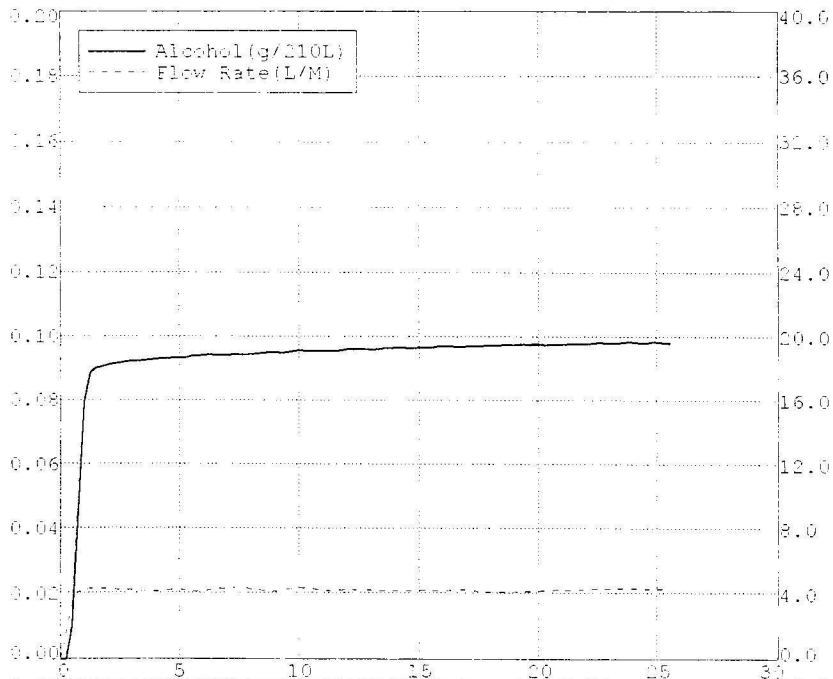

614