

SUPERVISOR TEST




SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 09/03/2022

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:54
INTERNAL STANDARD	VERIFIED	16:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:54
BLANK TEST	0.00	16:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:55
BLANK TEST	0.00	16:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:56
BLANK TEST	0.00	16:57

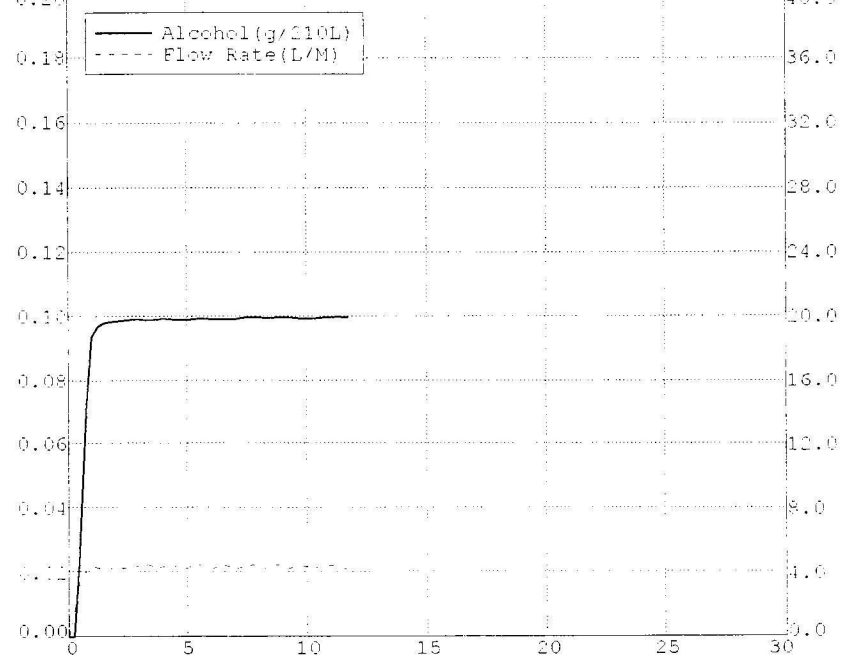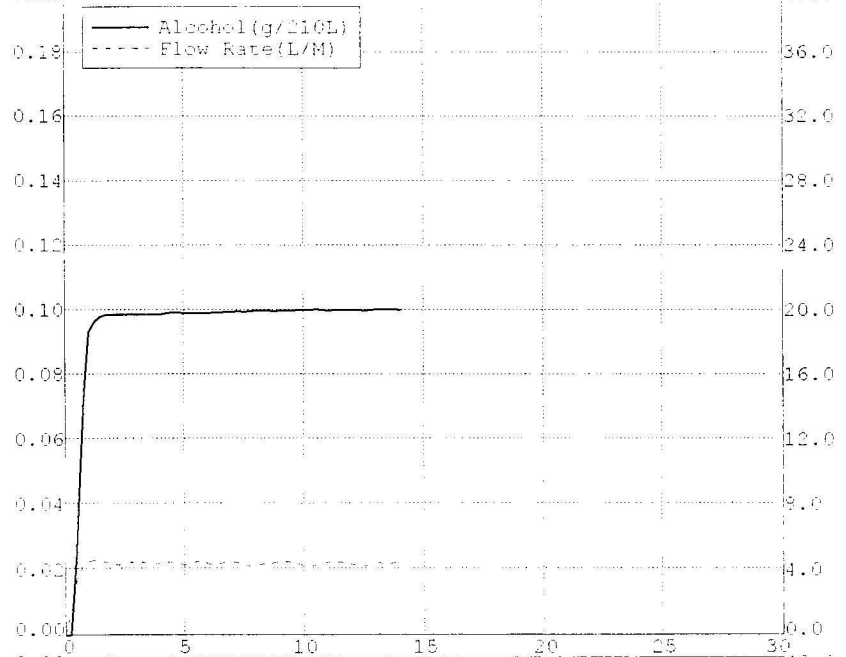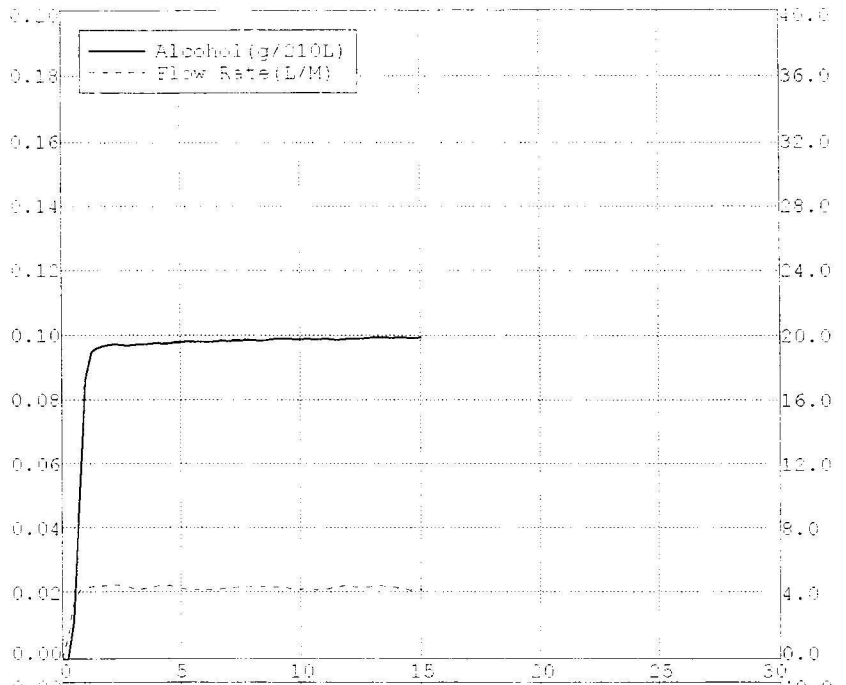

614