

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 09/05/2022

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:19
INTERNAL STANDARD	VERIFIED	15:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:19
BLANK TEST	0.00	15:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:20
BLANK TEST	0.00	15:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:22
BLANK TEST	0.00	15:23

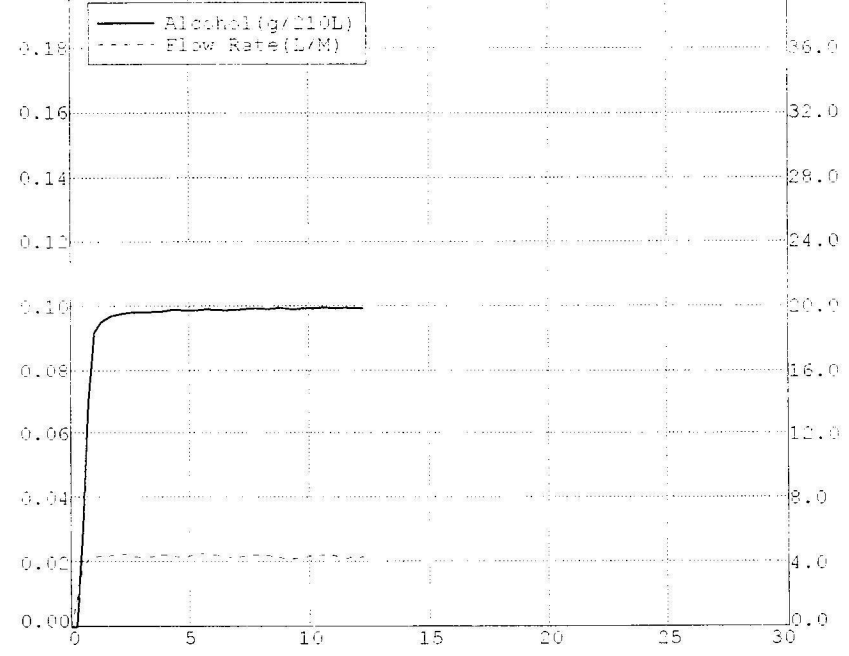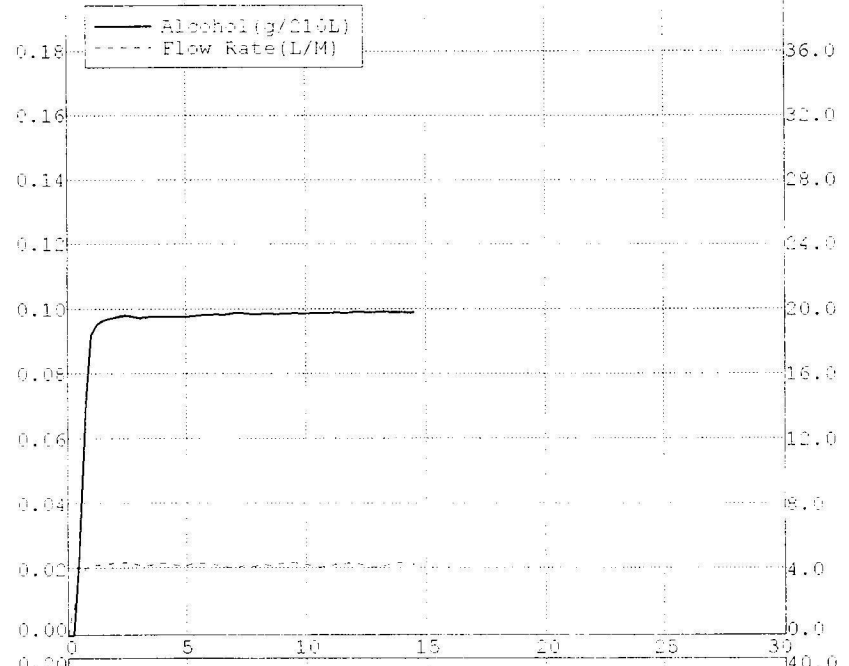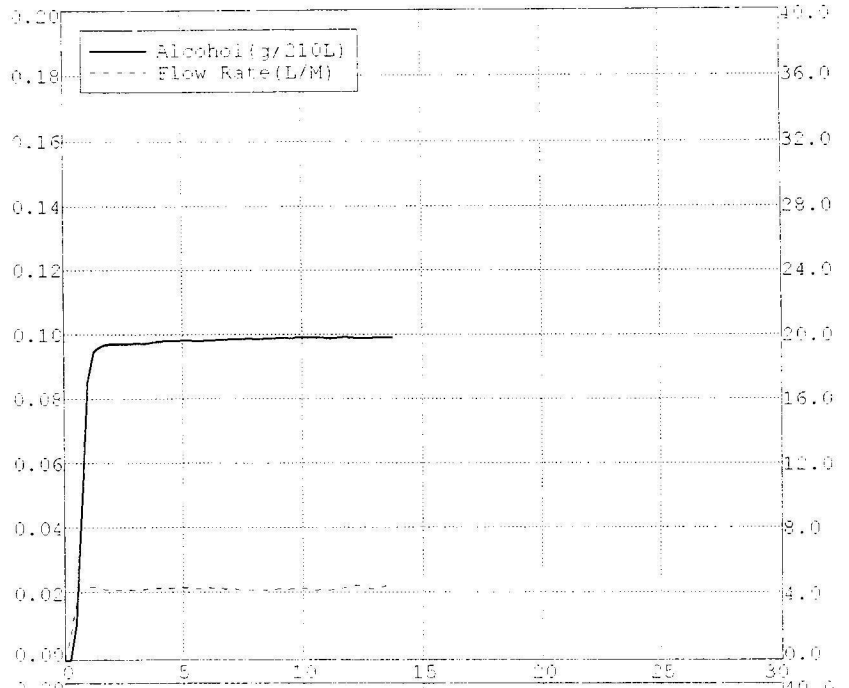

6/4