

SUPERVISOR TEST




-----  
SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106  
-----

Date: 09/12/2022

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:39
INTERNAL STANDARD	VERIFIED	08:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:40
BLANK TEST	0.00	08:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:41
BLANK TEST	0.00	08:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:42
BLANK TEST	0.00	08:43

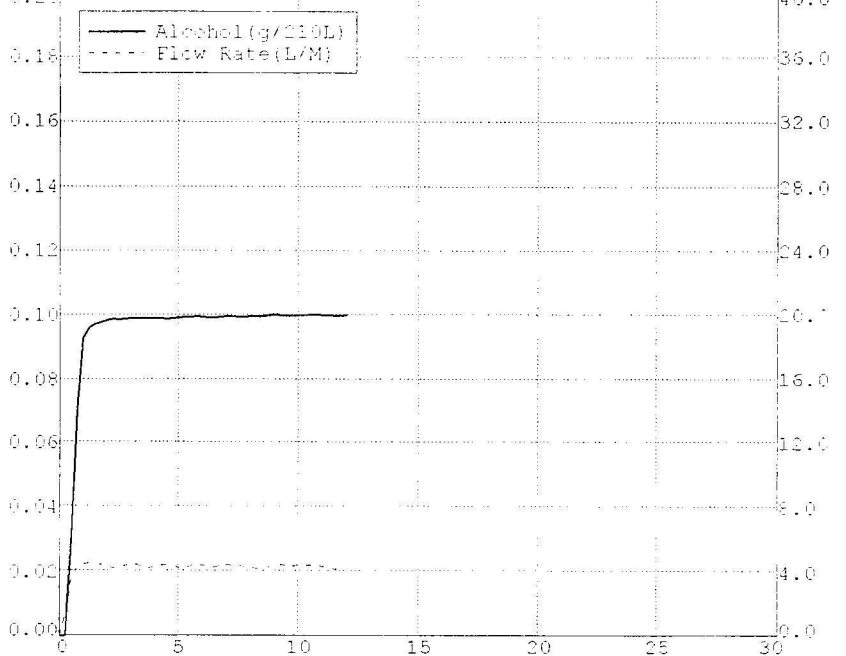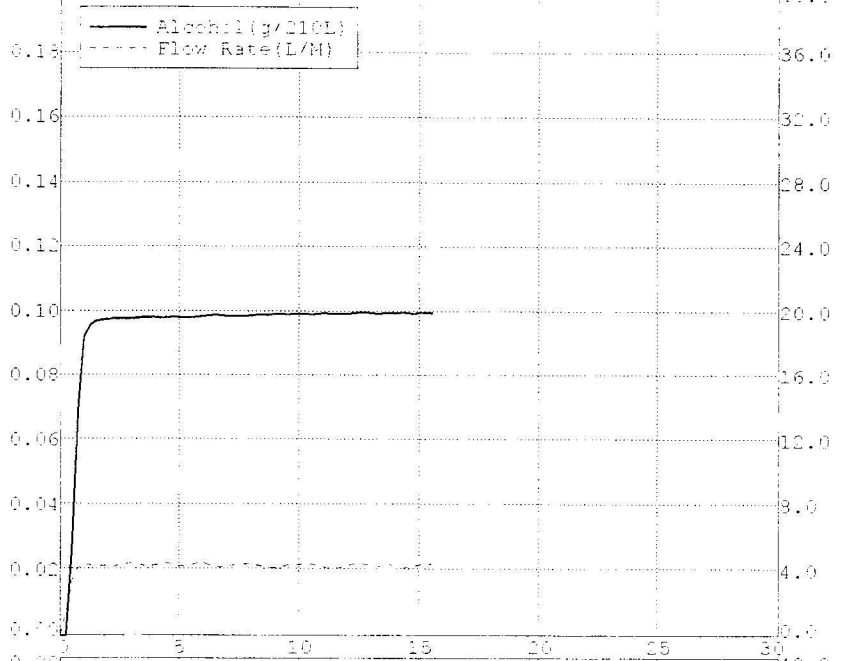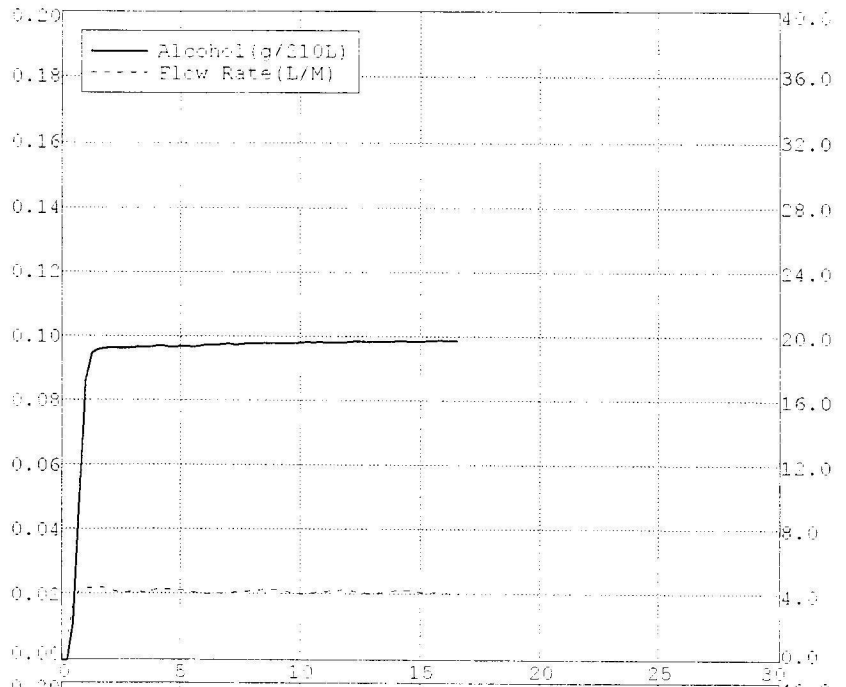

614