

SUPERVISOR TEST




SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 09/19/2022

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:50
INTERNAL STANDARD	VERIFIED	18:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:51
BLANK TEST	0.00	18:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:52
BLANK TEST	0.00	18:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:53
BLANK TEST	0.00	18:54

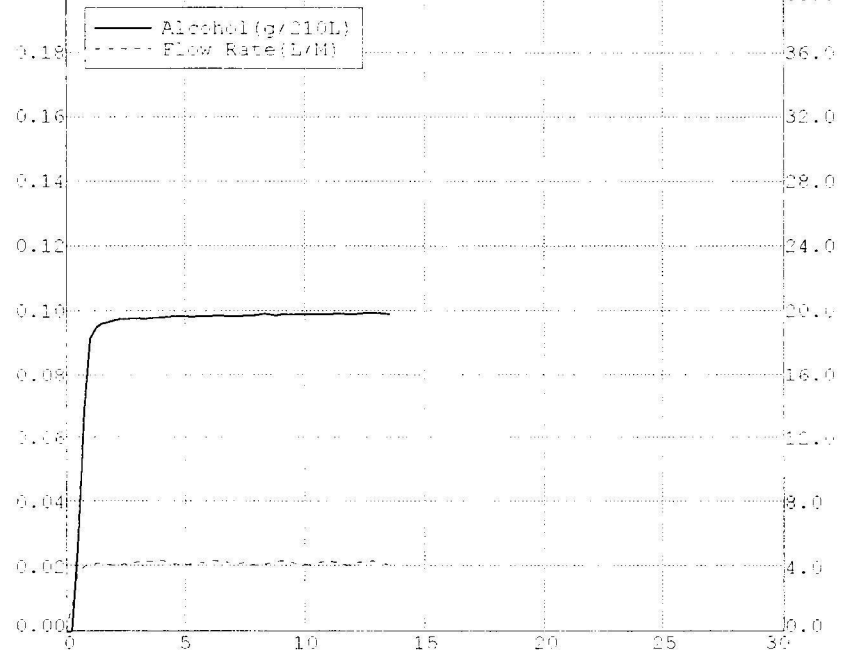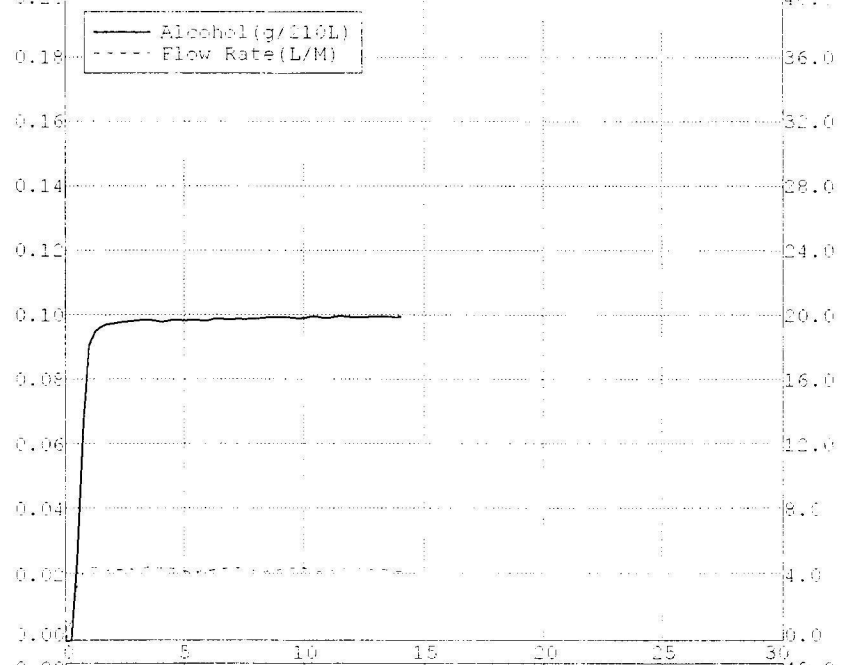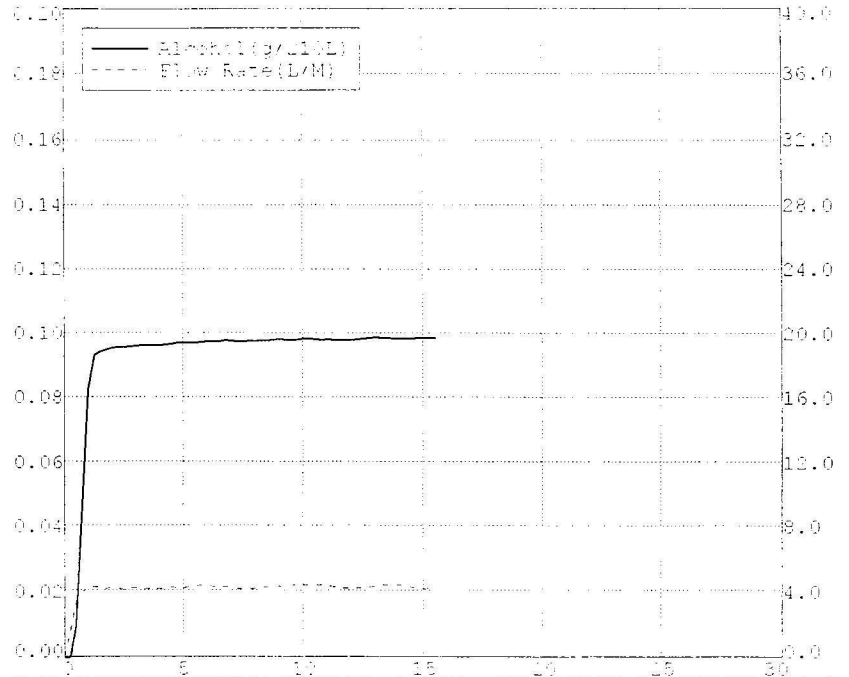

614