

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 09/26/2022

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:10
INTERNAL STANDARD	VERIFIED	08:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:10
BLANK TEST	0.00	08:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:11
BLANK TEST	0.00	08:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:13
BLANK TEST	0.00	08:14

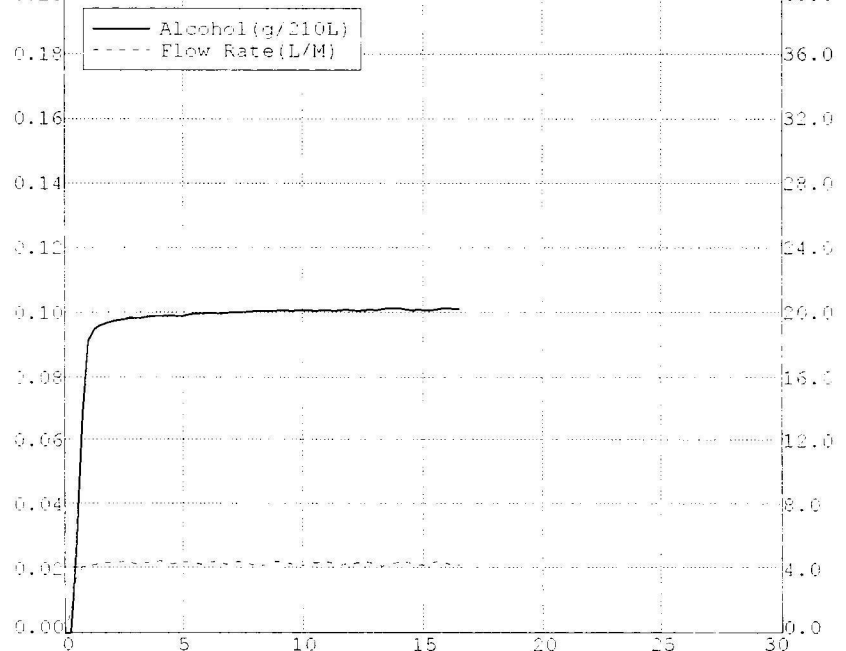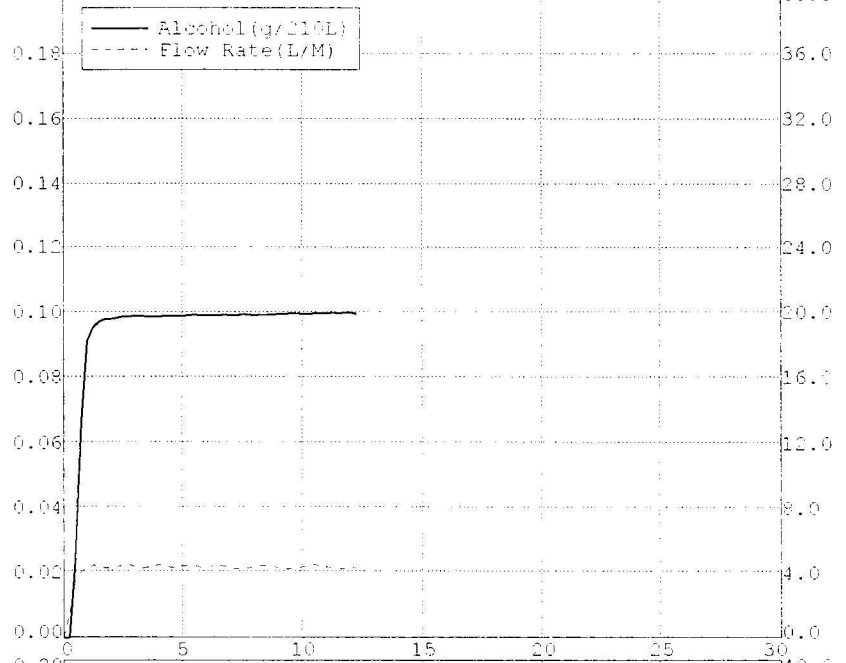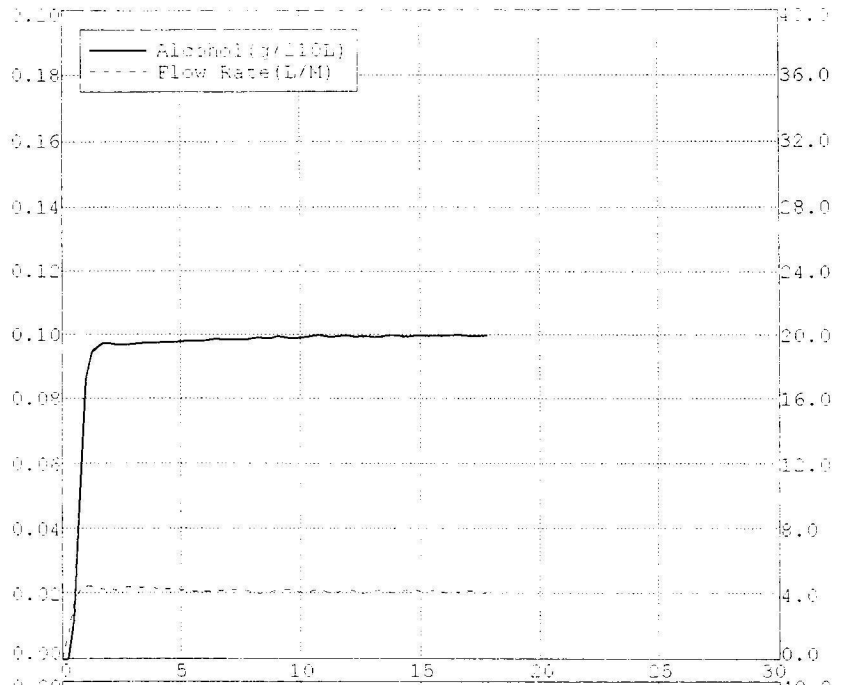

614