

SOLUTION CHANGE




SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 10/03/2022

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:25
INTERNAL STANDARD	VERIFIED	01:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:25
BLANK TEST	0.00	01:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:26
BLANK TEST	0.00	01:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:28
BLANK TEST	0.00	01:28

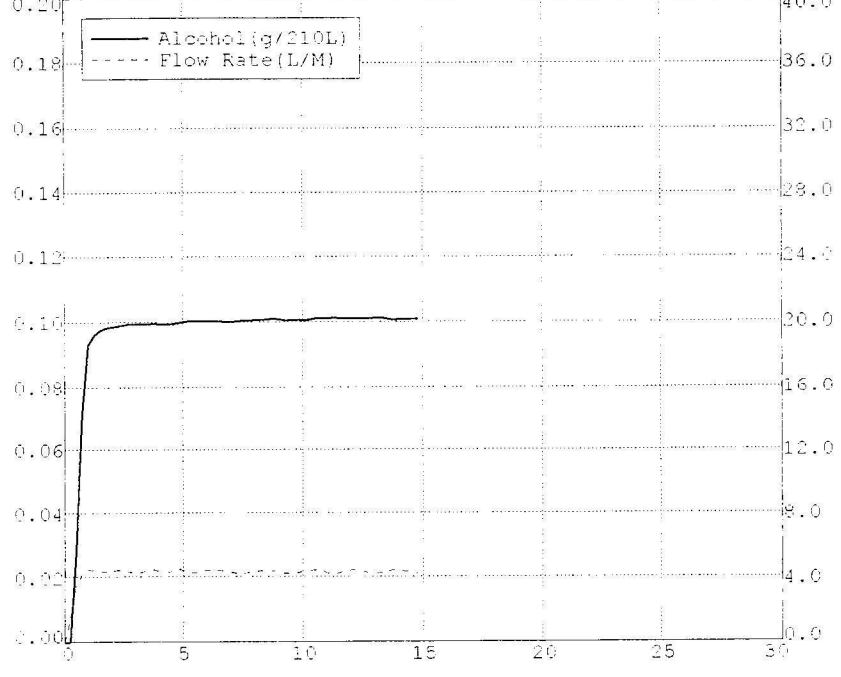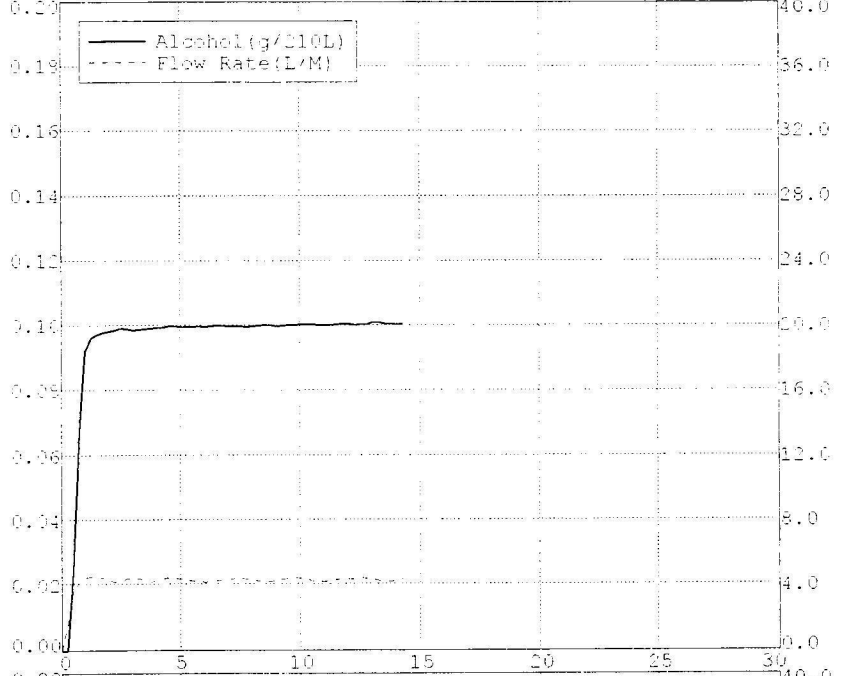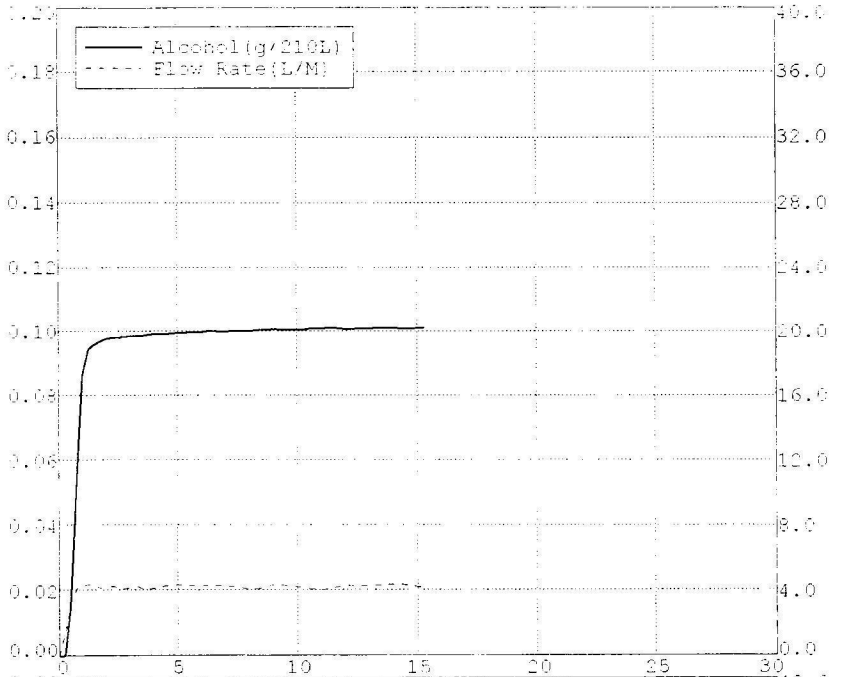

**ALCOHOL REFERENCE SOLUTION  
FOR SIMULATOR**

1181  
BOT. NO.

11/30/22  
EXP. DATE

22190  
LOT NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH  
A PROPERLY OPERATING BREATH SIMULATOR AND  
BREATH ALCOHOL ANALYZER, THE SOLUTION WILL  
PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.  
HARRISBURG, PENNSYLVANIA 17111

Rev. 1/06

614