

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 11/12/2022

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:22
INTERNAL STANDARD	VERIFIED	08:22
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	08:23
BLANK TEST	0.00	08:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:24
BLANK TEST	0.00	08:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:25
BLANK TEST	0.00	08:26

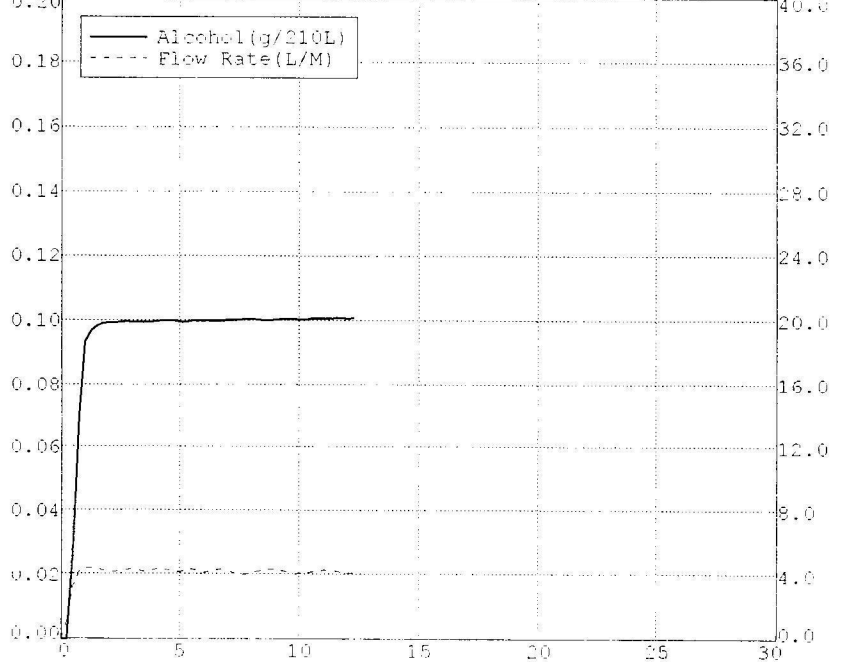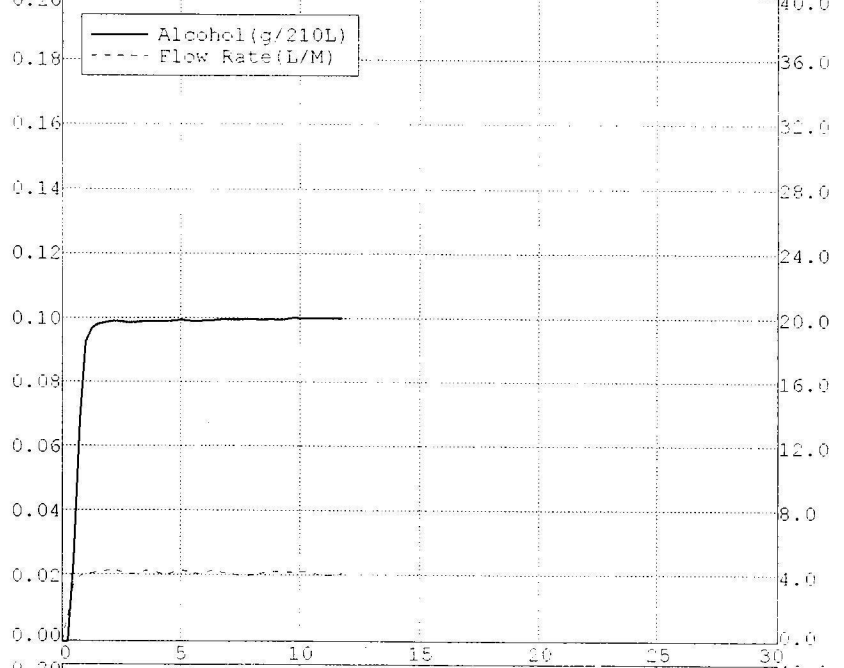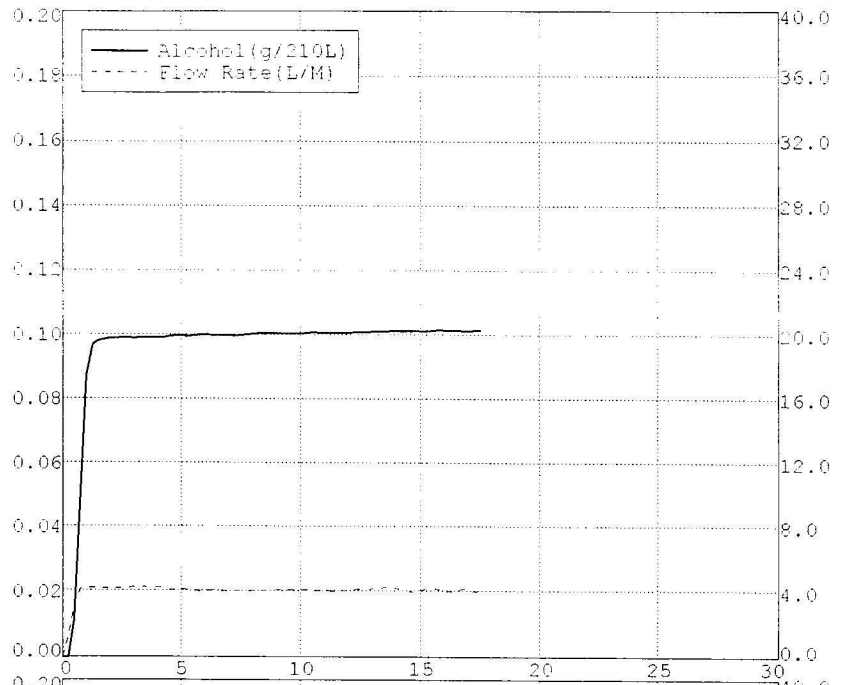

0614