

SUPERVISOR TEST




SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 11/14/2022

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:22
INTERNAL STANDARD	VERIFIED	08:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:23
BLANK TEST	0.00	08:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:24
BLANK TEST	0.00	08:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:25
BLANK TEST	0.00	08:26

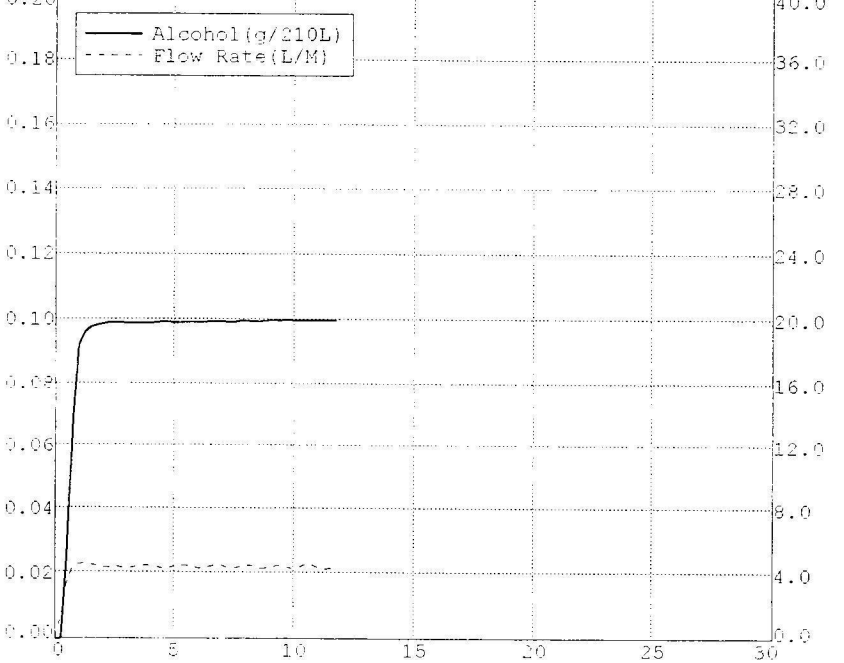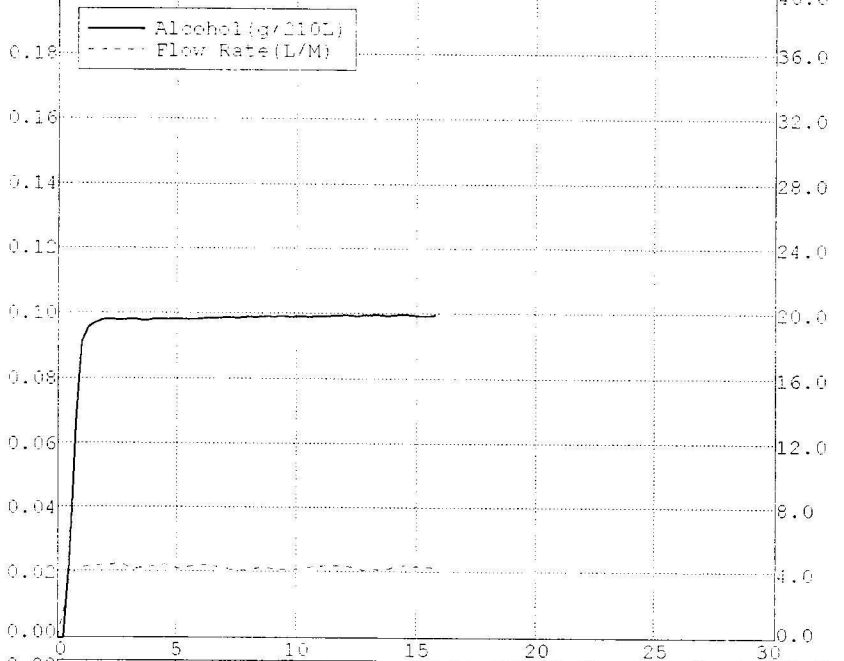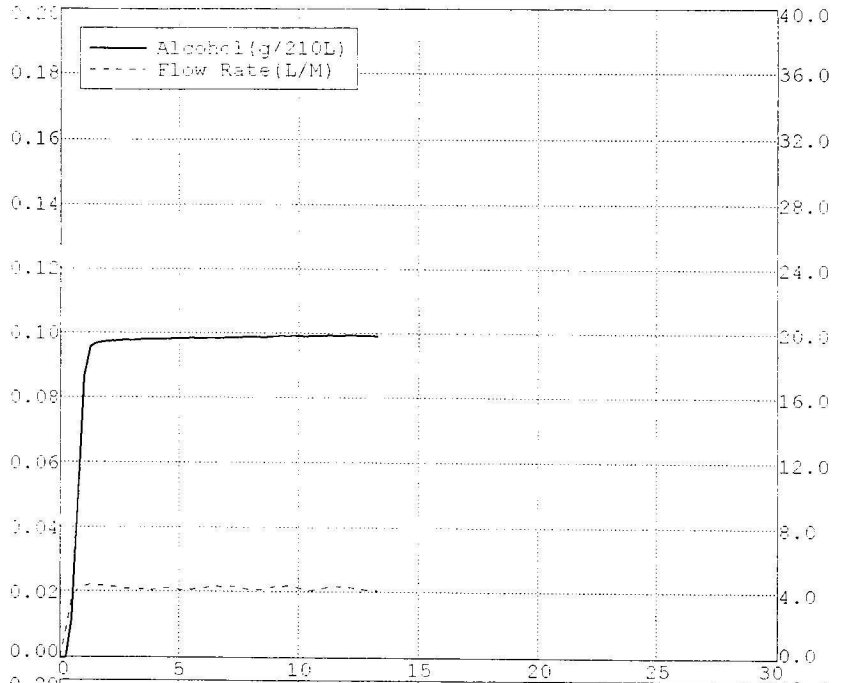

*Handwritten signature/initials*