

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 11/21/2022

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:20
INTERNAL STANDARD	VERIFIED	16:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:20
BLANK TEST	0.00	16:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:22
BLANK TEST	0.00	16:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:23
BLANK TEST	0.00	16:24

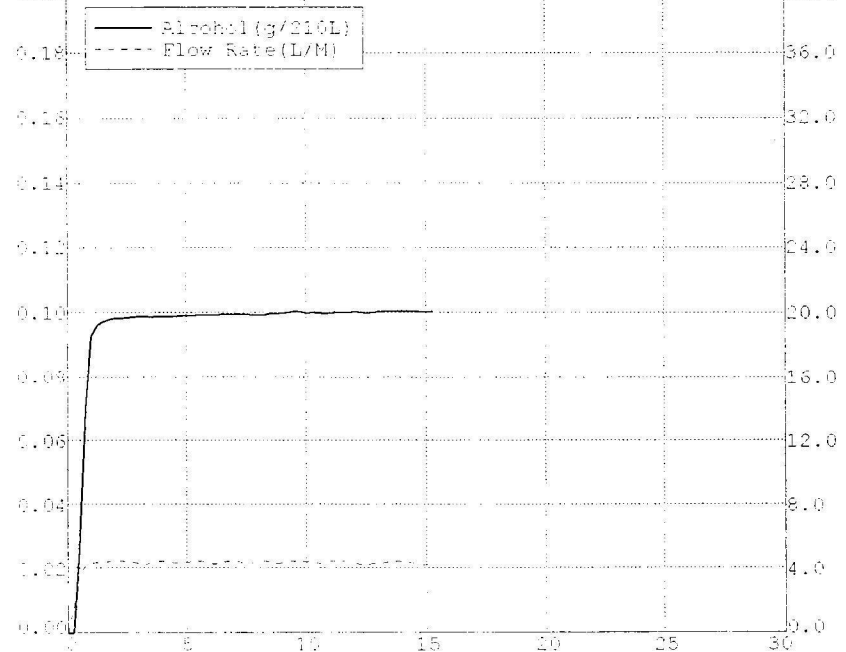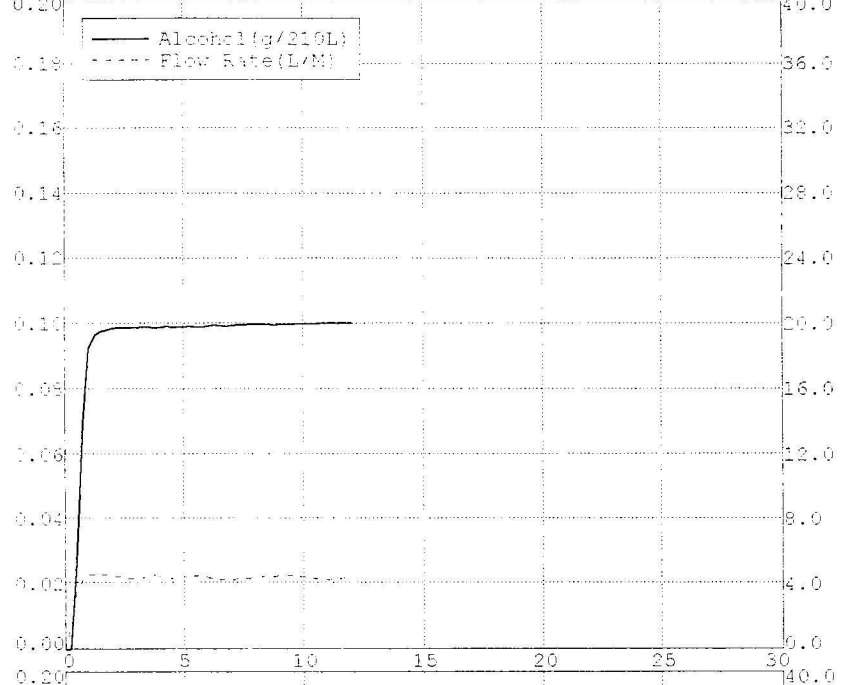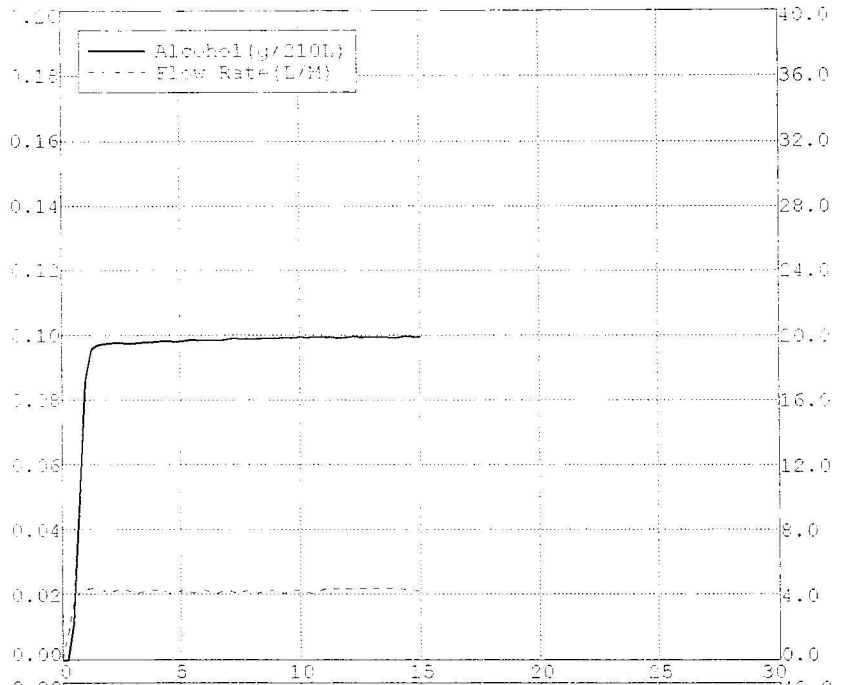

② 14