

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 11/28/2022

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22260

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 08:23 |
| INTERNAL STANDARD | VERIFIED | 08:23 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 08:24 |
| BLANK TEST | 0.00 | 08:25 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 08:25 |
| BLANK TEST | 0.00 | 08:26 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 08:26 |
| BLANK TEST | 0.00 | 08:27 |

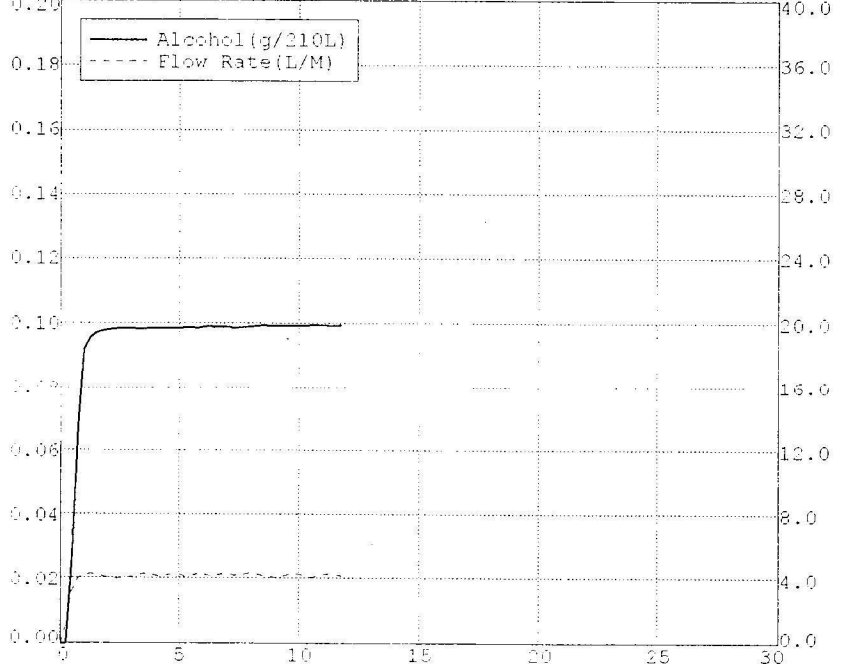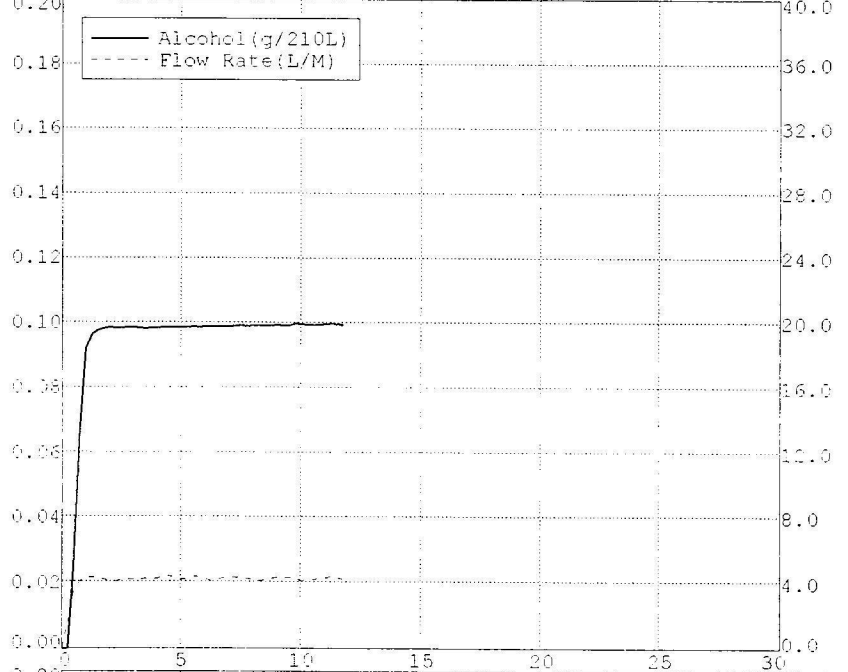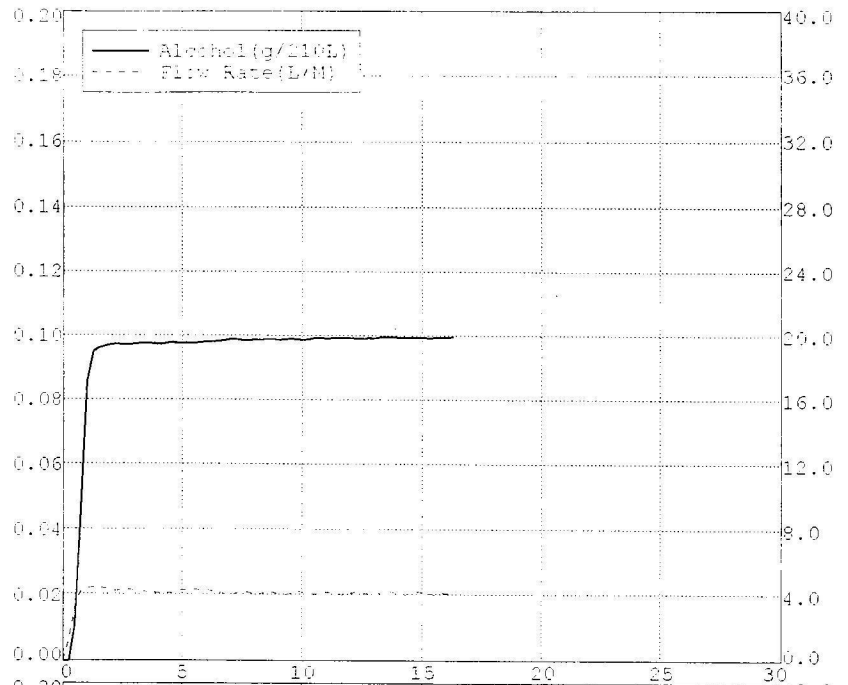

Handwritten signature and number 614