

SOLUTION CHANGE

SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 12/02/2022

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:41
INTERNAL STANDARD	VERIFIED	11:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:41
BLANK TEST	0.00	11:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:42
BLANK TEST	0.00	11:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:44
BLANK TEST	0.00	11:44

**ALCOHOL REFERENCE SOLUTION
 FOR SIMULATOR**

81
 BOT. NO.


3/27/23
 EXP. DATE

22390
 LOT NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH
 A PROPERLY OPERATING BREATH SIMULATOR AND
 BREATH ALCOHOL ANALYZER, THE SOLUTION WILL
 PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.
 HARRISBURG, PENNSYLVANIA 17111

Rev. 1/06

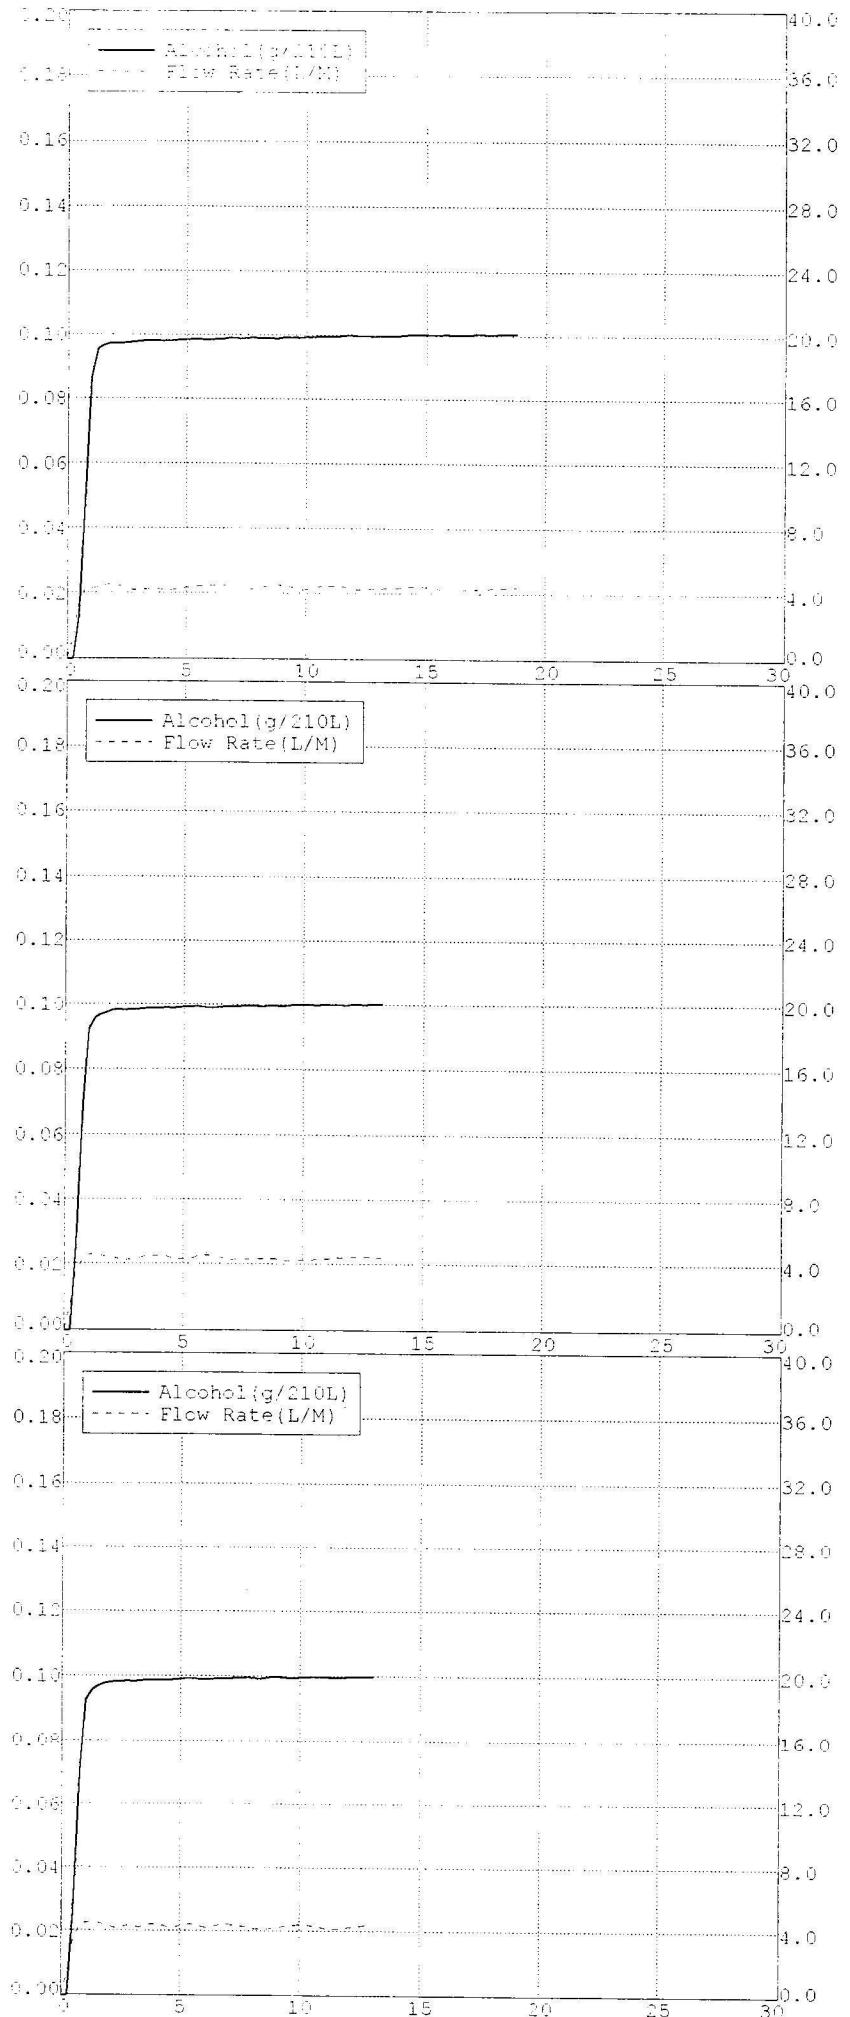

614