

SOLUTION CHANGE

SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 01/02/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:37
INTERNAL STANDARD	VERIFIED	18:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:37
BLANK TEST	0.00	18:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:38
BLANK TEST	0.00	18:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:40
BLANK TEST	0.00	18:41

ALCOHOL REFERENCE SOLUTION
FOR SIMULATOR

22390
LOT NO.




3/27/23
EXP. DATE

249
BOT. NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH
A PROPERLY OPERATING BREATH SIMULATOR AND
BREATH ALCOHOL ANALYZER, THE SOLUTION WILL
PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.
HARRISBURG, PENNSYLVANIA 17111

Rev. 1/06

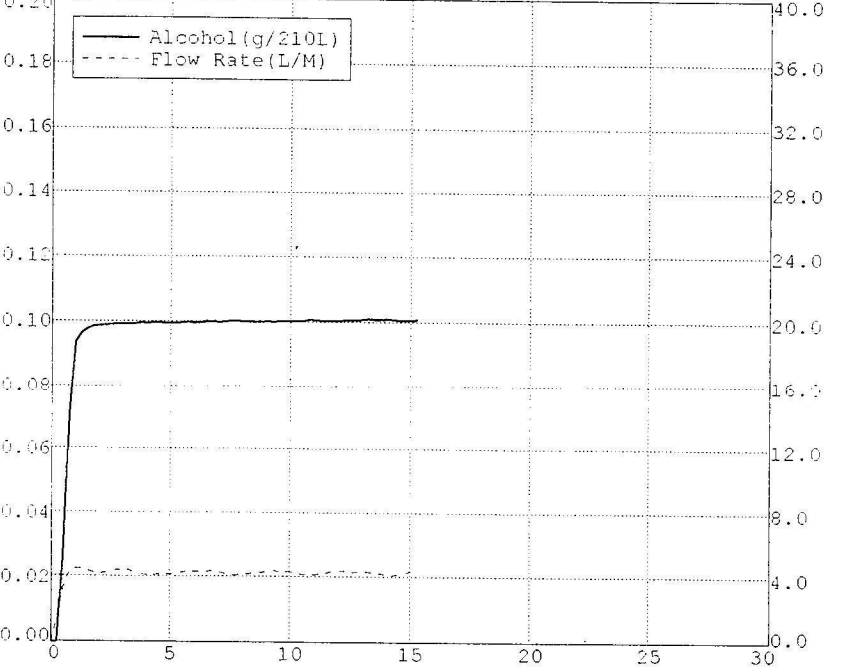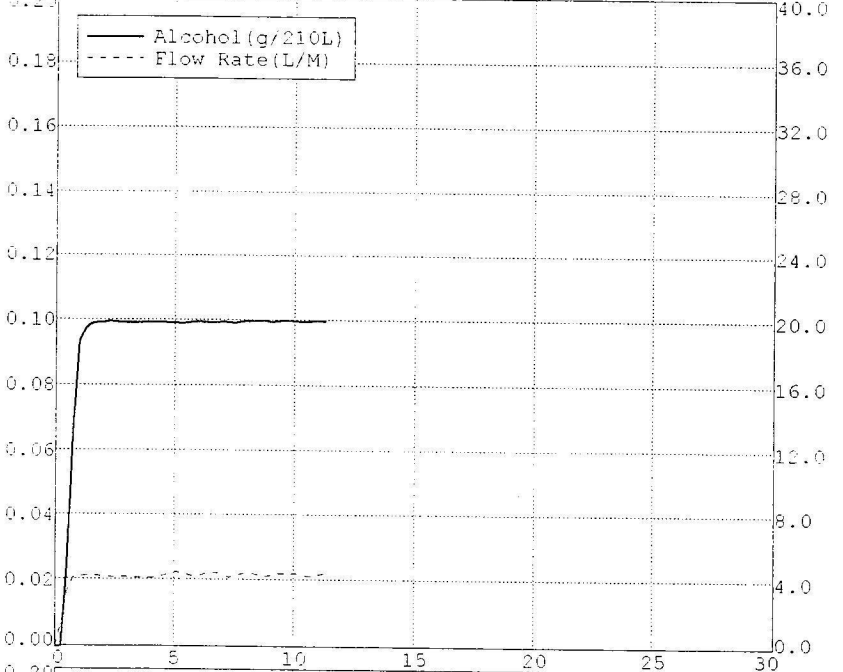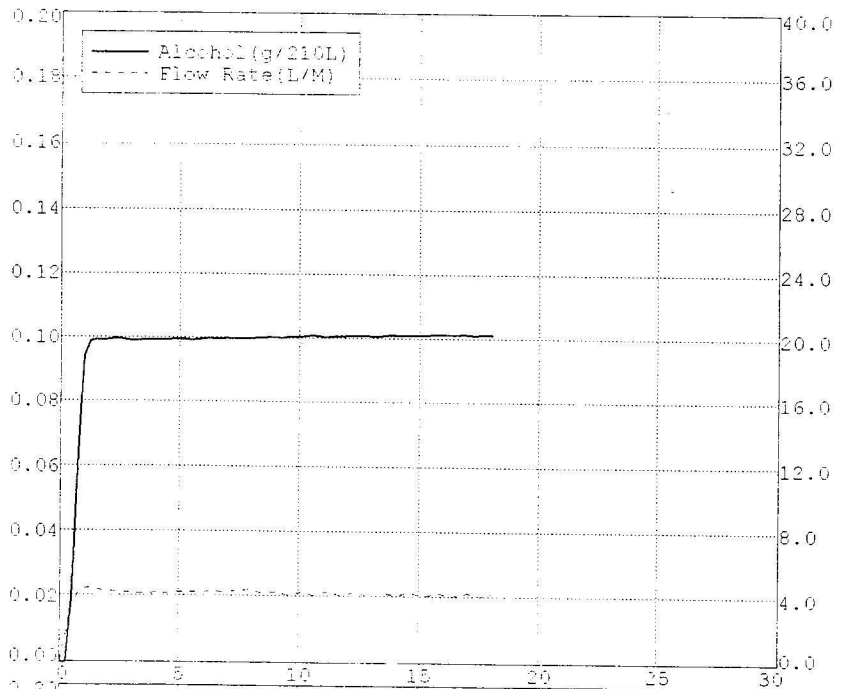

614

SOLUTION CHANGE

SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106


Date: 01/02/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:44
INTERNAL STANDARD	VERIFIED	16:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:45

Blank Error

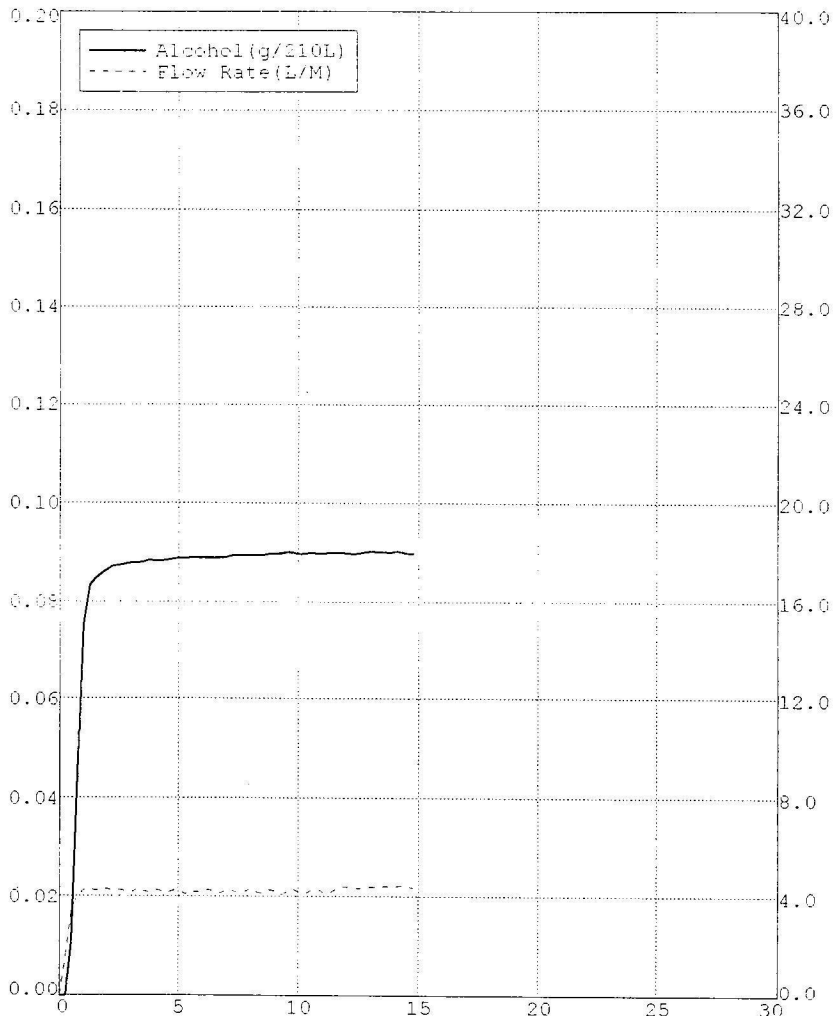

2614