

SOLUTION CHANGE

SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 02/01/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:32
INTERNAL STANDARD	VERIFIED	00:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:33
BLANK TEST	0.00	00:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:34
BLANK TEST	0.00	00:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:35
BLANK TEST	0.00	00:36


ALCOHOL REFERENCE SOLUTION
FOR SIMULATOR

22420 LOT NO.
5/23/23 EXP. DATE
1126 BOT. NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH
A PROPERLY OPERATING BREATH SIMULATOR AND
BREATH ALCOHOL ANALYZER, THE SOLUTION WILL
PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.
HARRISBURG, PENNSYLVANIA 17111

Rev. 1/06

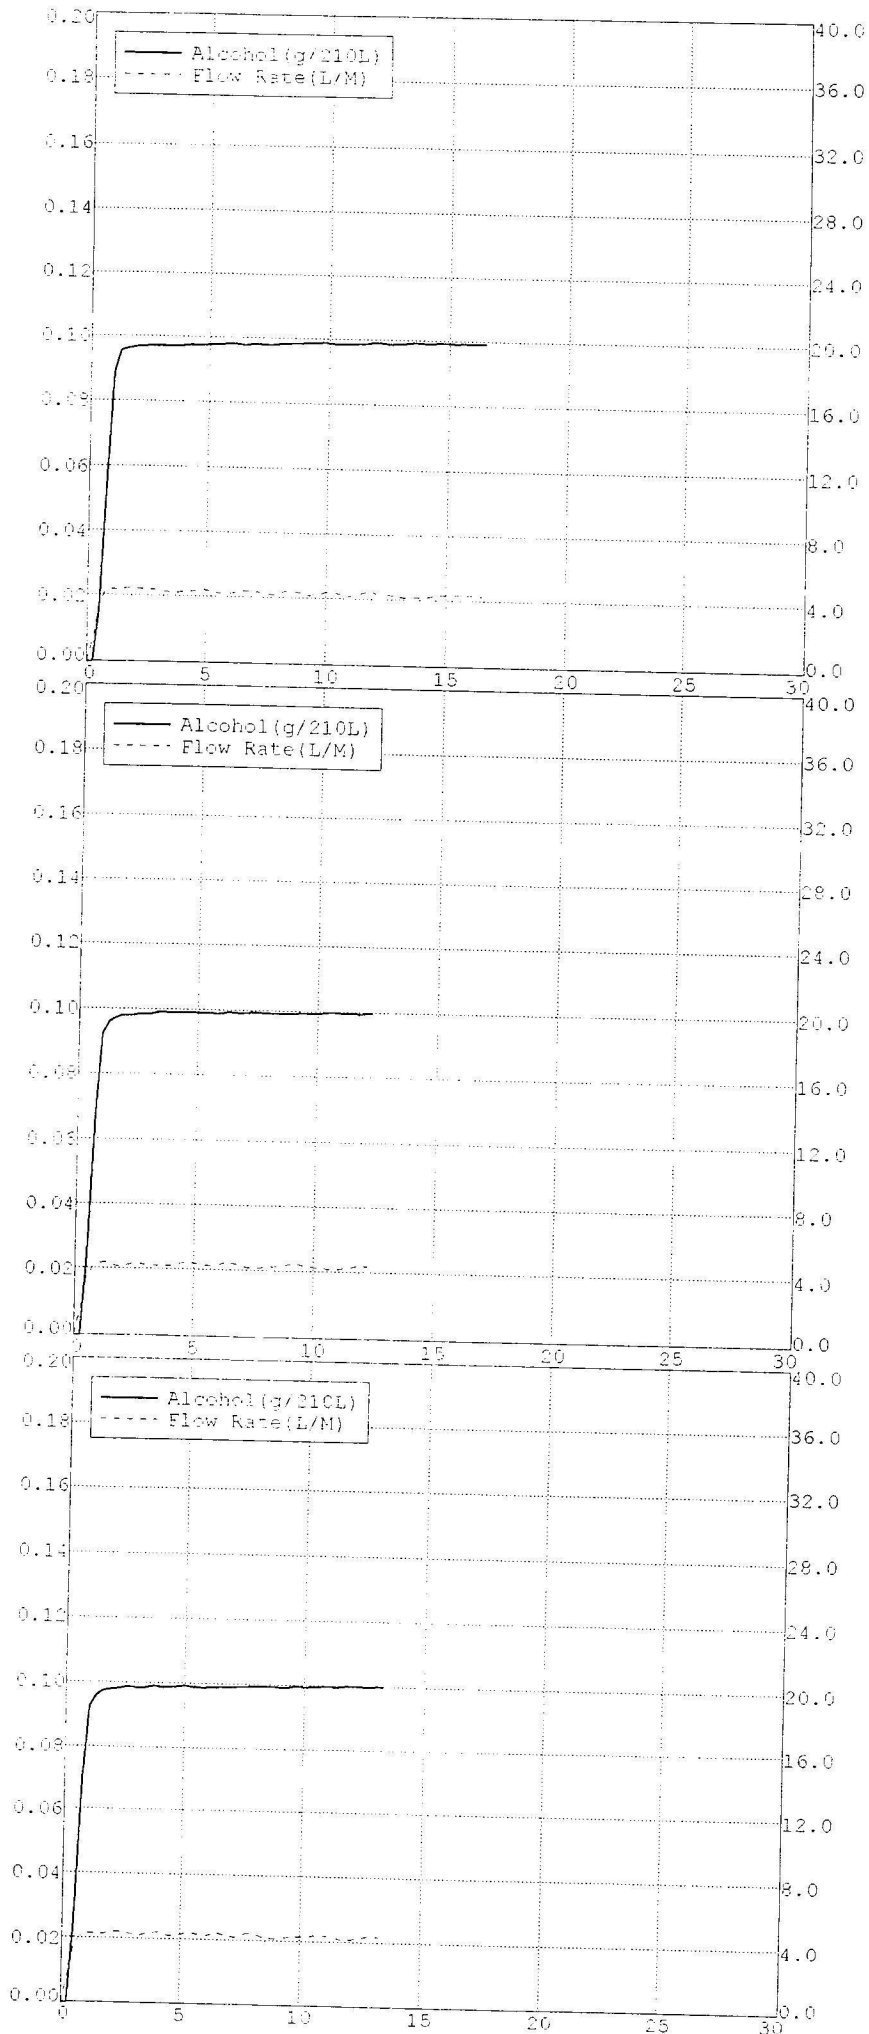

614