

SUPERVISOR TEST




-----  
SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106  
-----

Date: 02/08/2023

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:09
INTERNAL STANDARD	VERIFIED	08:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:10
BLANK TEST	0.00	08:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:11
BLANK TEST	0.00	08:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:12
BLANK TEST	0.00	08:13

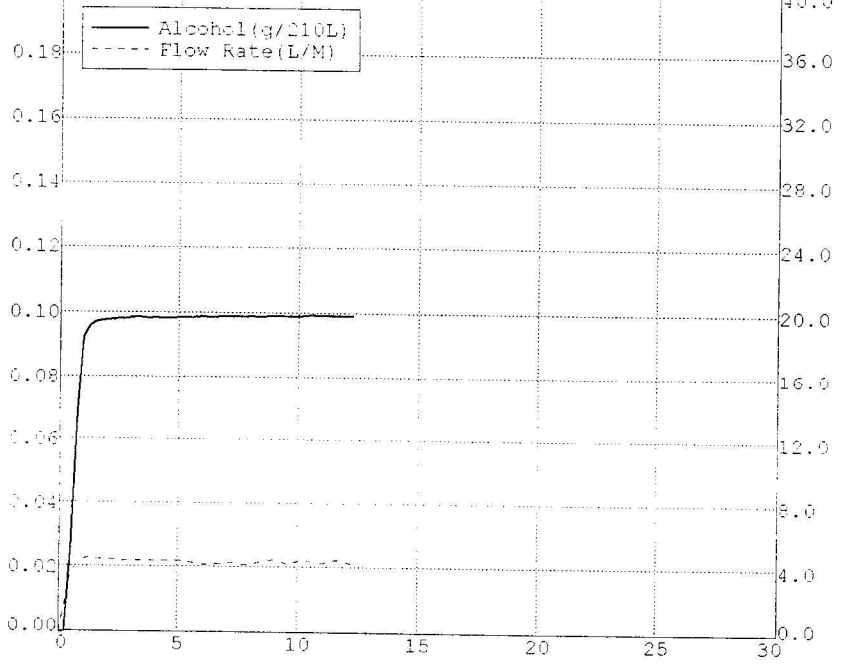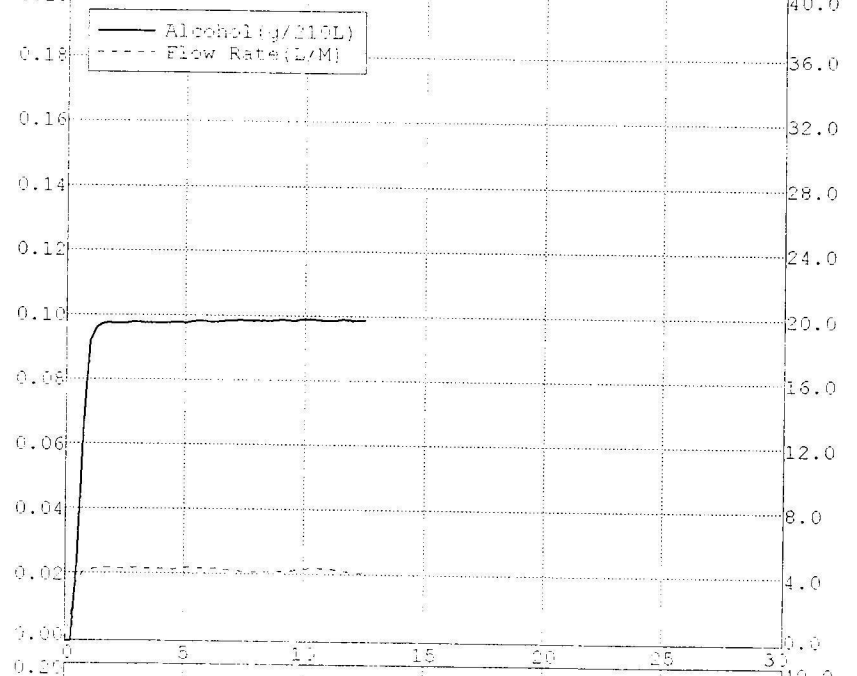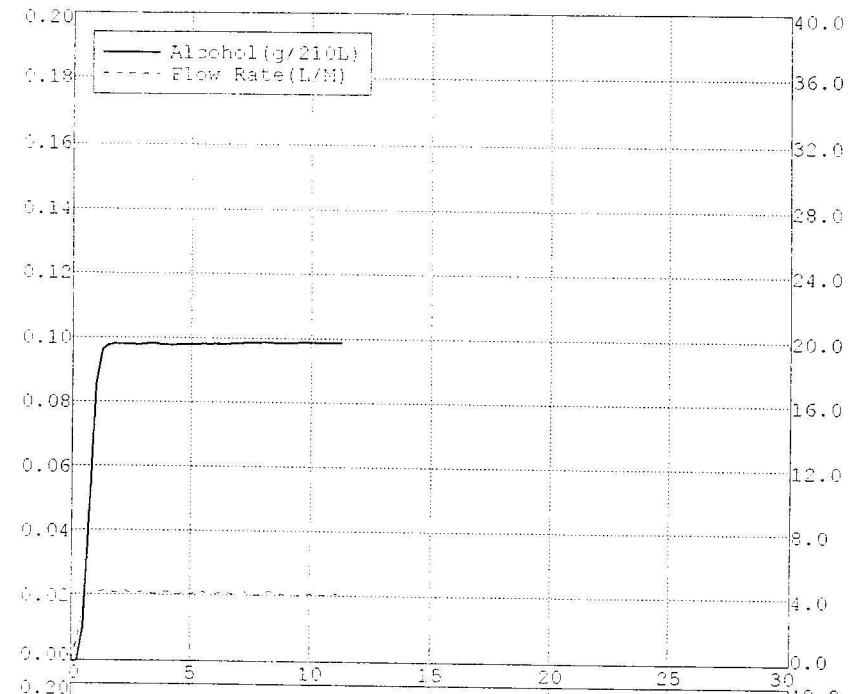

610