

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 02/15/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:13
INTERNAL STANDARD	VERIFIED	16:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:14
BLANK TEST	0.00	16:15
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	16:15
BLANK TEST	0.00	16:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:16
BLANK TEST	0.00	16:17

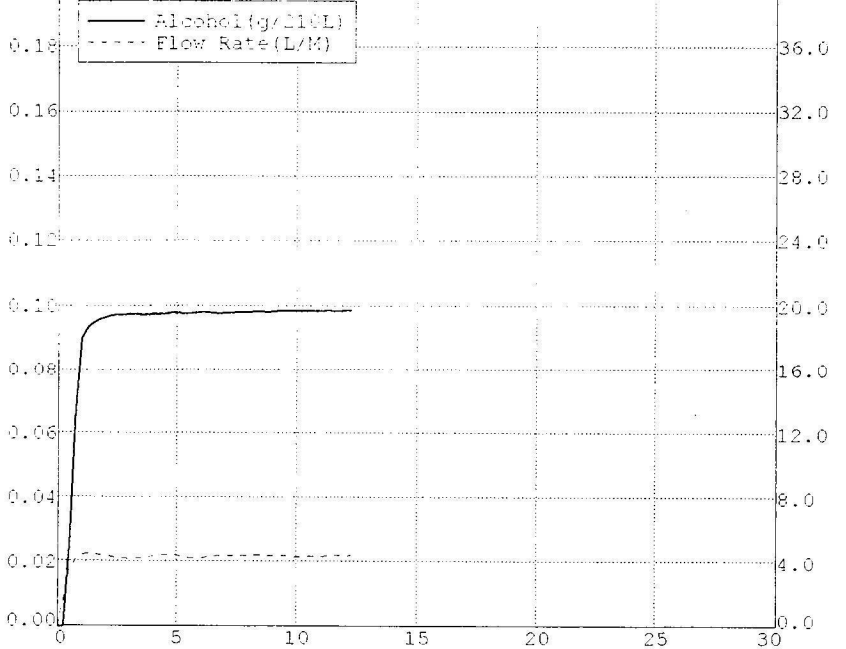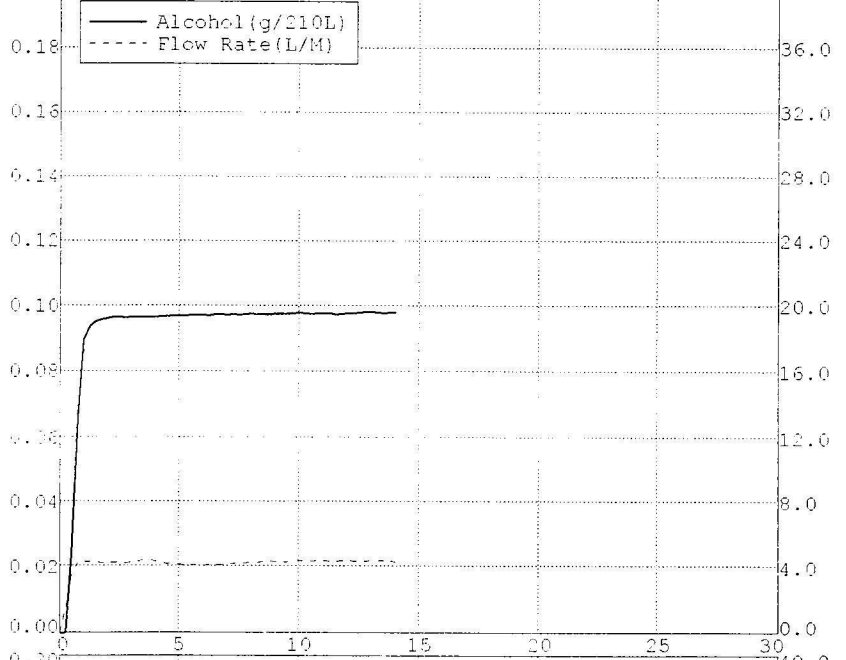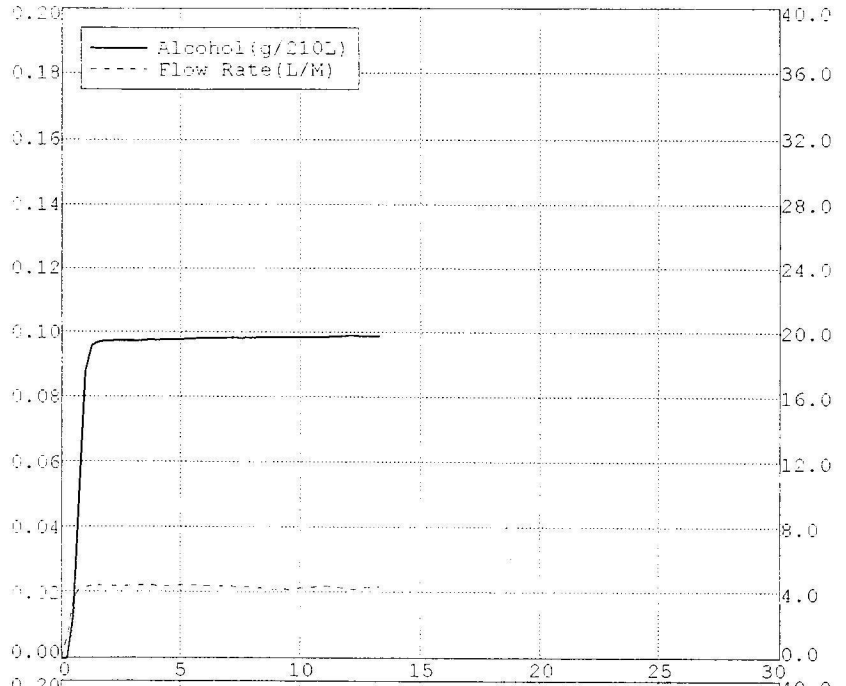

614