

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 02/18/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:03
INTERNAL STANDARD	VERIFIED	19:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:03
BLANK TEST	0.00	19:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:05
BLANK TEST	0.00	19:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:06
BLANK TEST	0.00	19:07

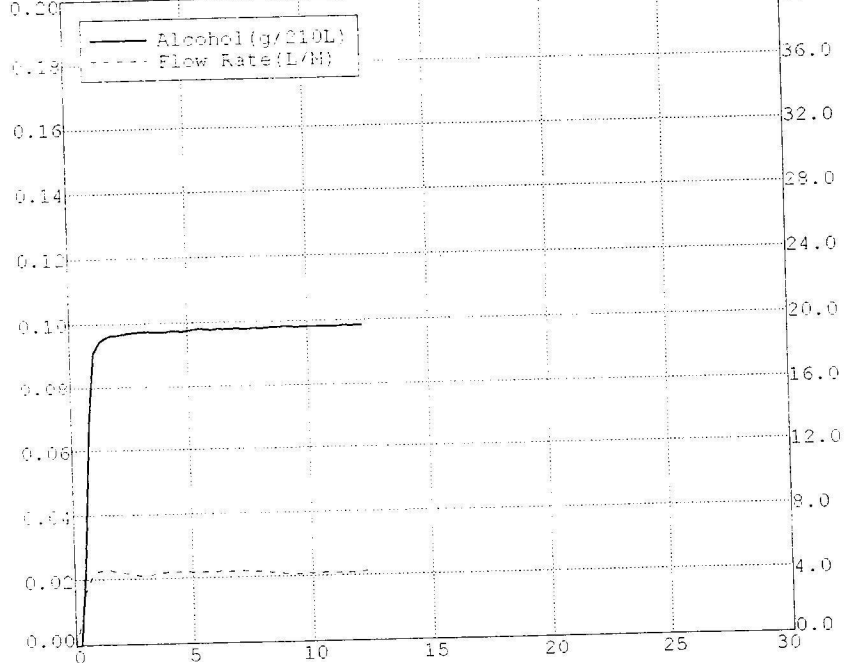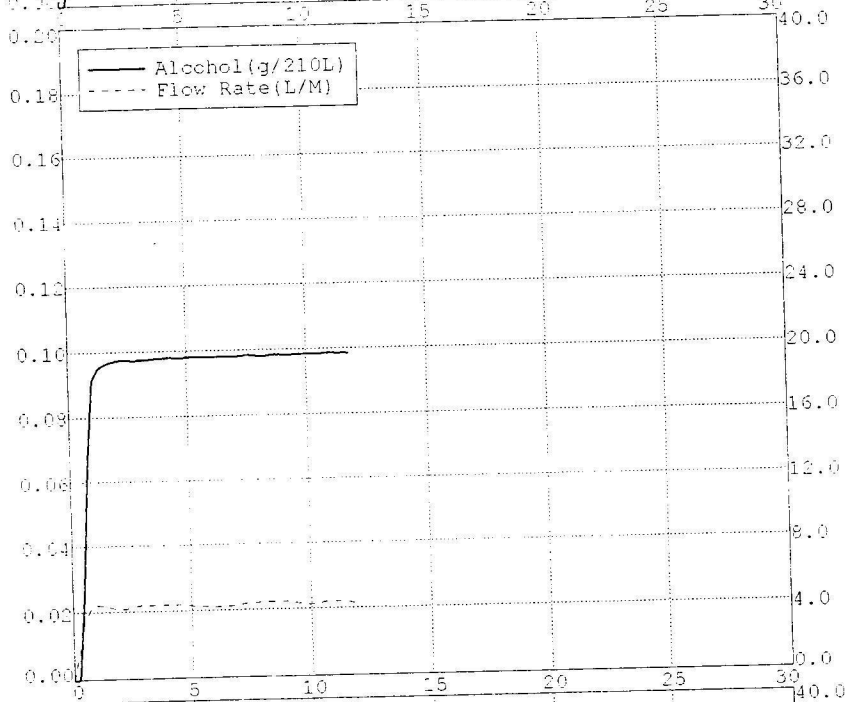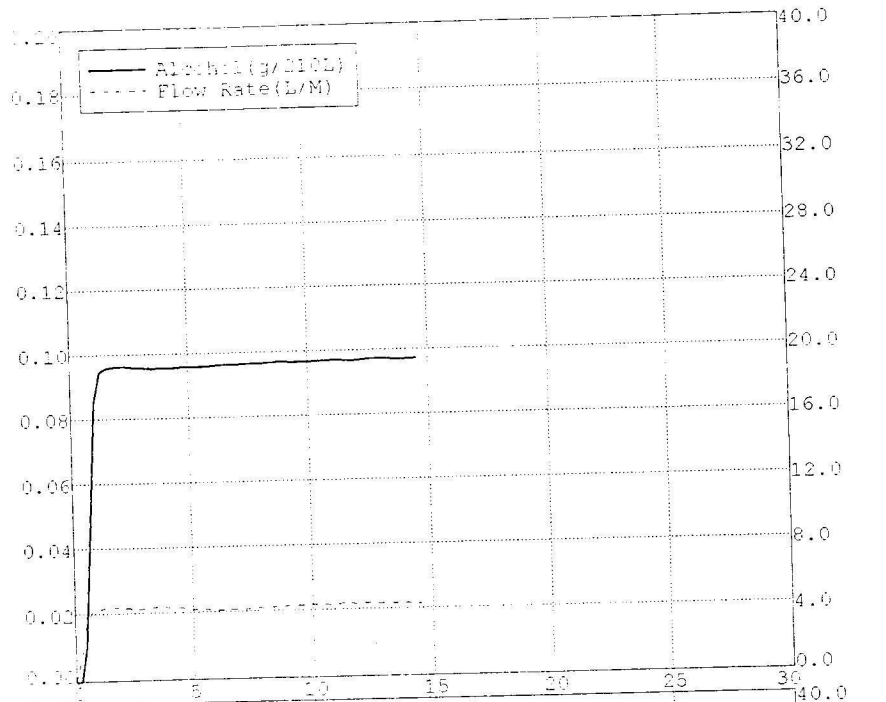

614