

SOLUTION CHANGE

-----  
 SPRING VALLEY VILLAGE  
 POLICE DEPT  
 DATAMASTER dmt: 127106  
 -----

Date: 03/03/2023

OPERATOR NAME:  
 BRANDON KING  
 Permit #: 36388  
 Operator Agency/Dept: SPRING VALLEY PD  
 Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:34
INTERNAL STANDARD	VERIFIED	00:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:35
BLANK TEST	0.00	00:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:36
BLANK TEST	0.00	00:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:37
BLANK TEST	0.00	00:38

ALCOHOL REFERENCE SOLUTION  
FOR SIMULATOR

1291  
BOT. NO.




5/23/23  
EXP. DATE

22420  
LOT NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH  
 A PROPERLY OPERATING BREATH SIMULATOR AND  
 BREATH ALCOHOL ANALYZER, THE SOLUTION WILL  
 PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.  
 HARRISBURG, PENNSYLVANIA 17111

Rev. 1/06

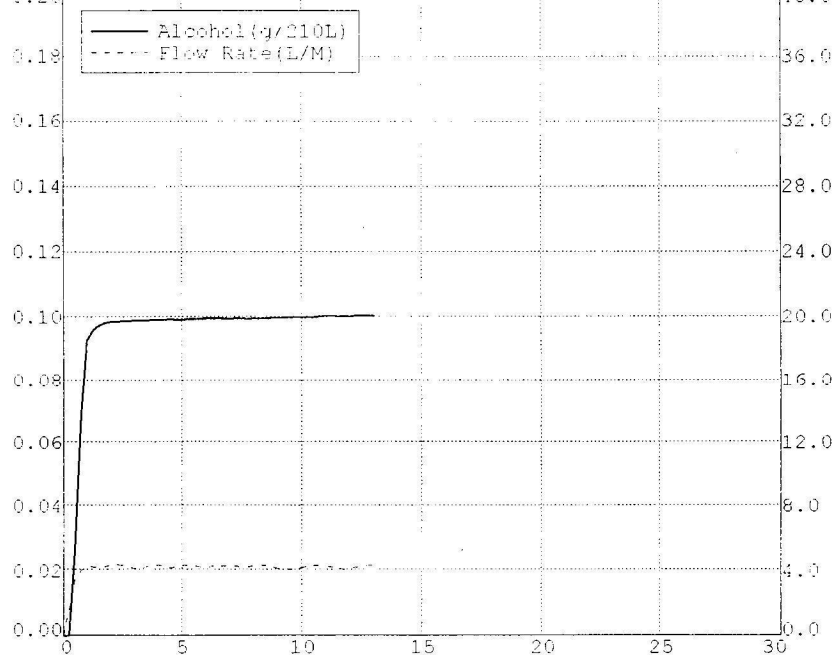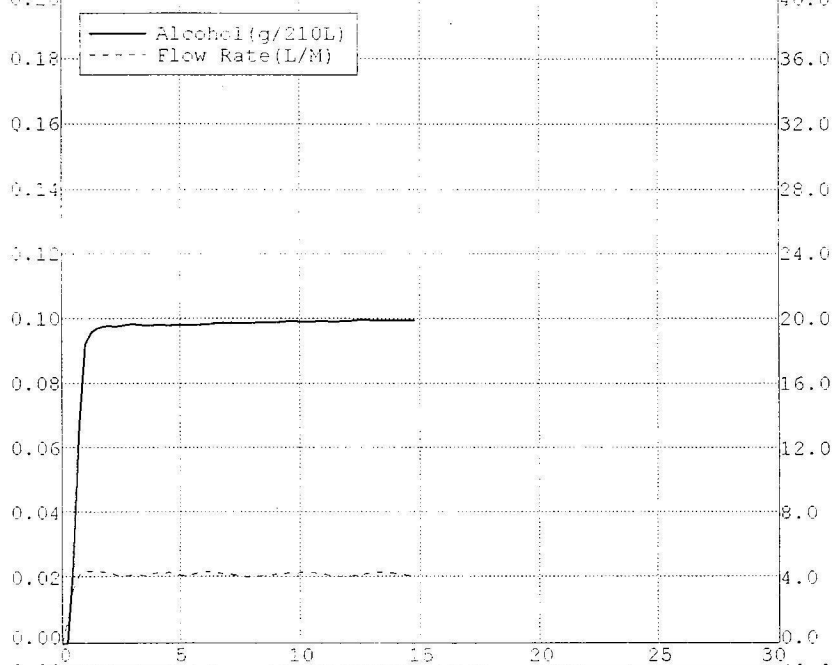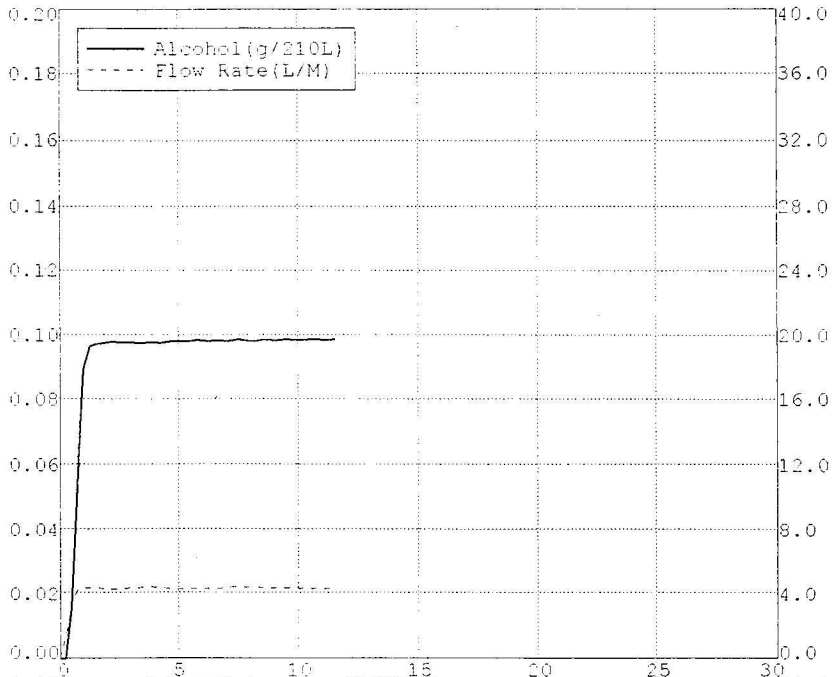

614