

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 03/20/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:34
INTERNAL STANDARD	VERIFIED	20:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:34
BLANK TEST	0.00	20:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:35
BLANK TEST	0.00	20:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:37
BLANK TEST	0.00	20:38

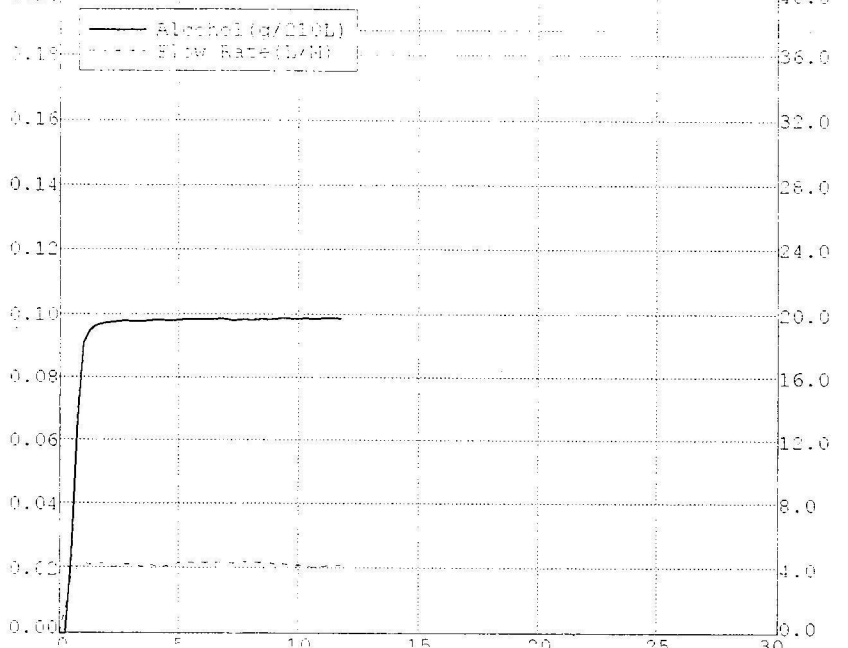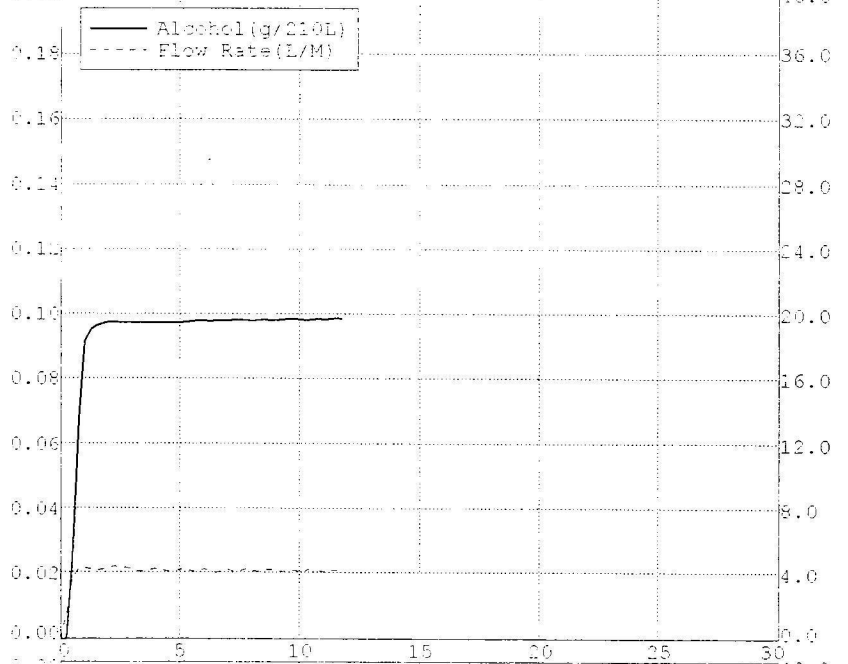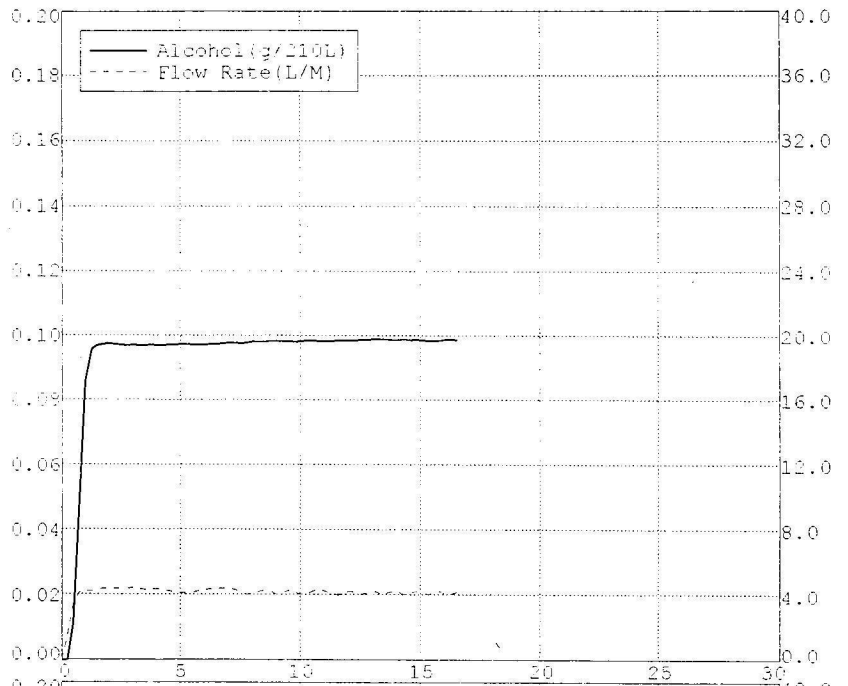

0614