

SOLUTION CHANGE

SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 04/01/2023

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:36
INTERNAL STANDARD	VERIFIED	16:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:36
BLANK TEST	0.00	16:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:37
BLANK TEST	0.00	16:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:38
BLANK TEST	0.00	16:39

ALCOHOL REFERENCE SOLUTION  
FOR SIMULATOR

1301  
BOT. NO.




7/24/23  
EXP. DATE

23030  
LOT NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH  
A PROPERLY OPERATING BREATH SIMULATOR AND  
BREATH ALCOHOL ANALYZER, THE SOLUTION WILL  
PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.  
HARRISBURG, PENNSYLVANIA 17111

Rev. 1/06

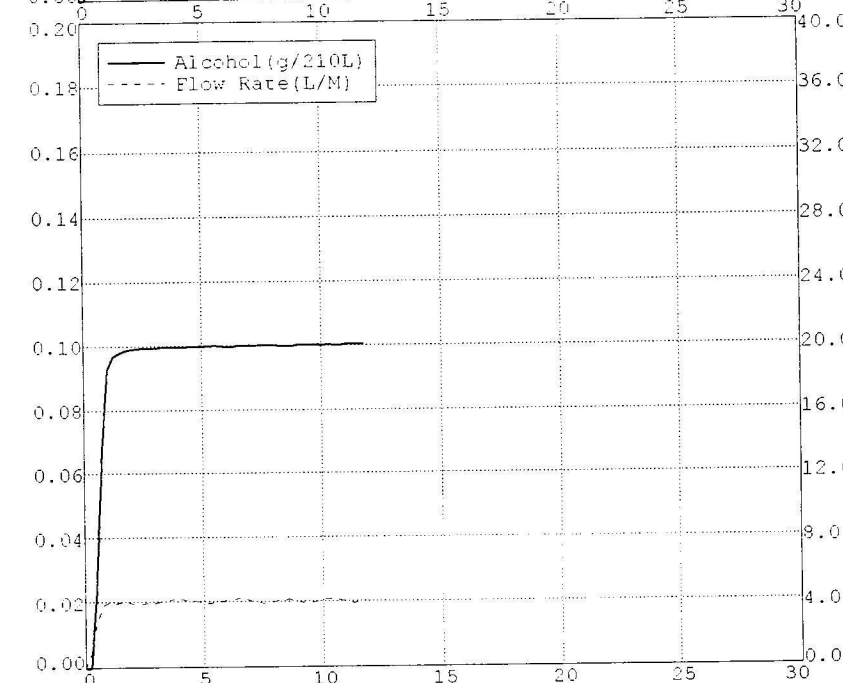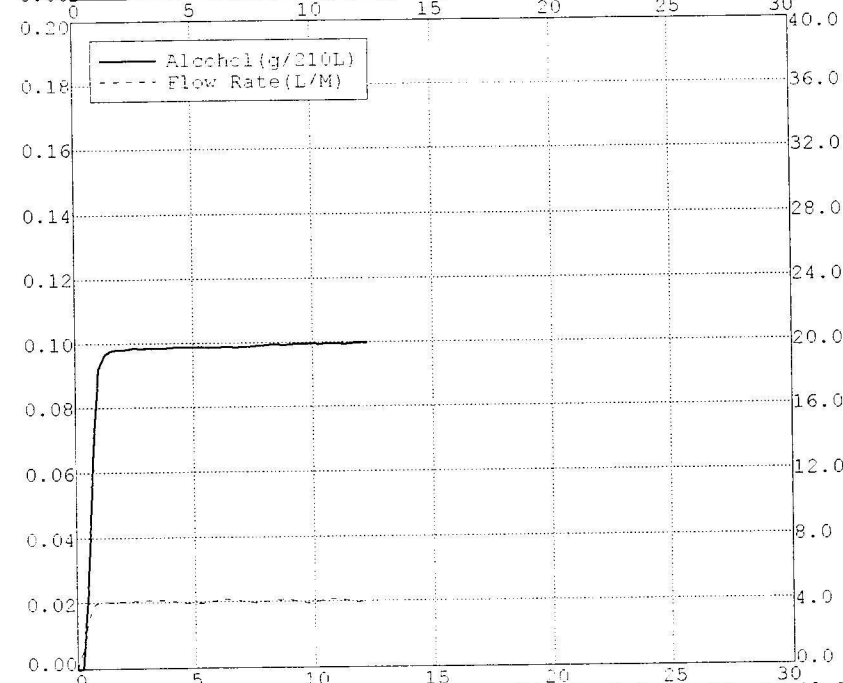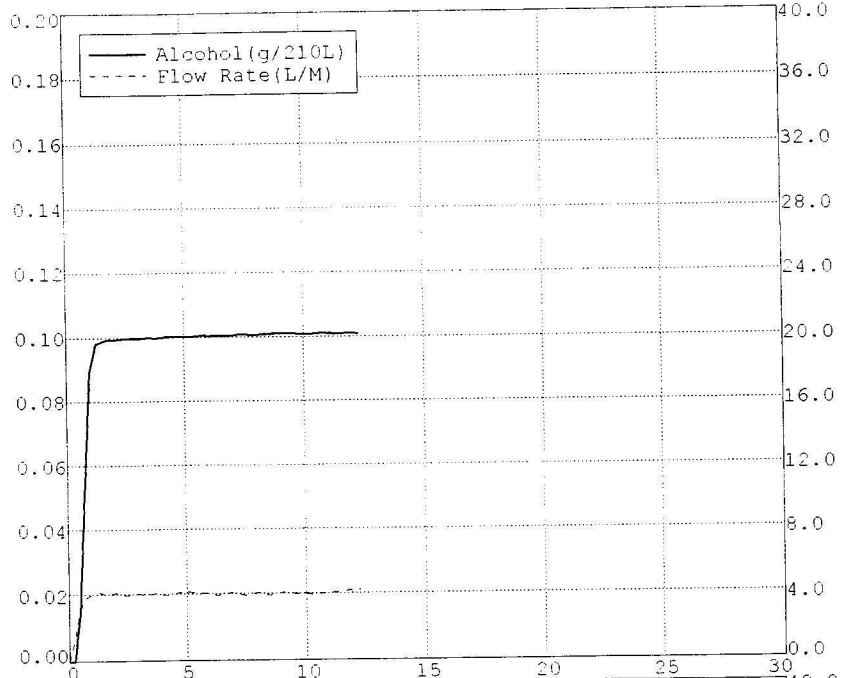

614