

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 05/20/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:13
INTERNAL STANDARD	VERIFIED	02:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:14
BLANK TEST	0.00	02:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:15
BLANK TEST	0.00	02:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:17
BLANK TEST	0.00	02:18

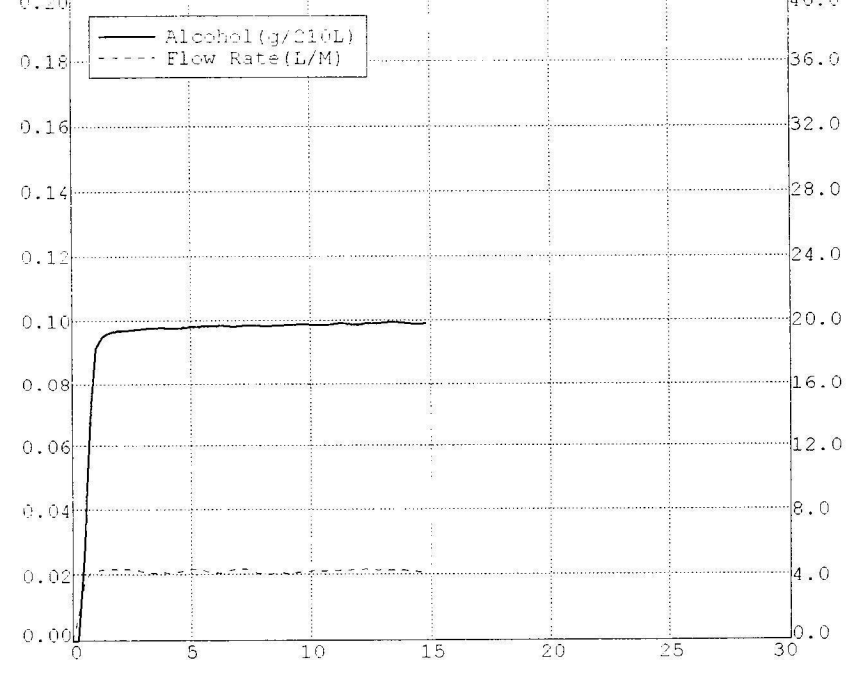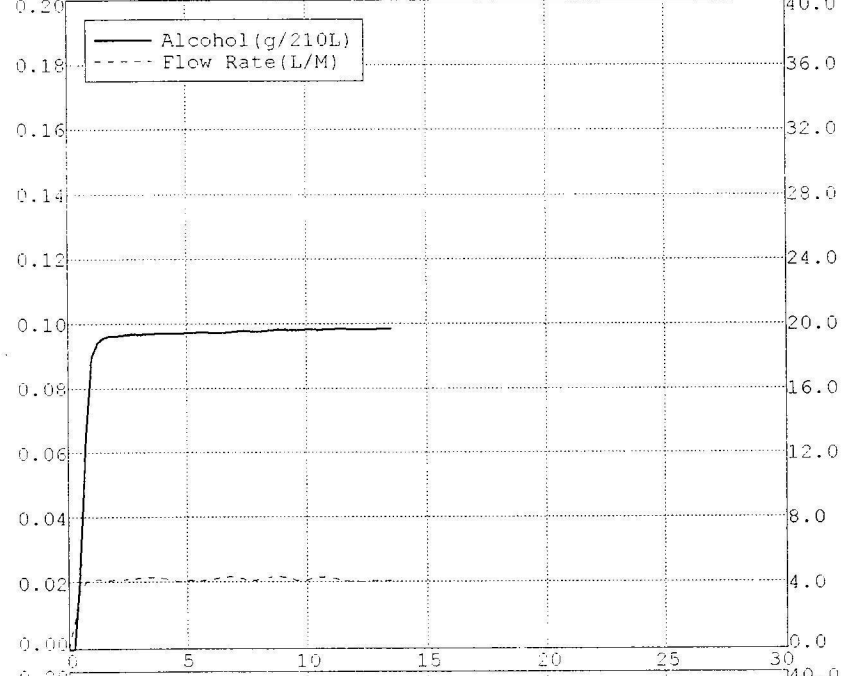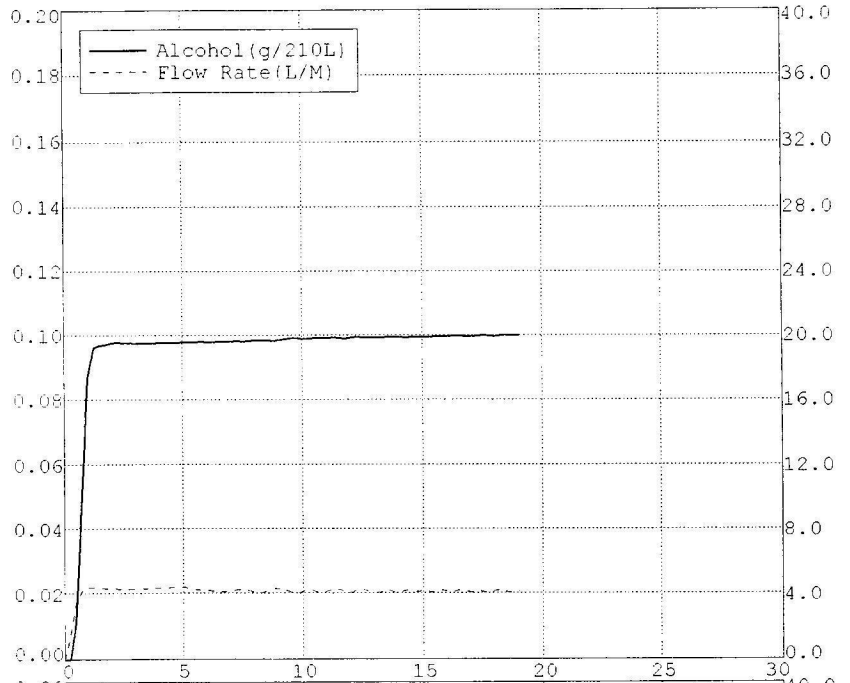

2614