

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 05/24/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:07
INTERNAL STANDARD	VERIFIED	08:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:08
BLANK TEST	0.00	08:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:09
BLANK TEST	0.00	08:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:10
BLANK TEST	0.00	08:11

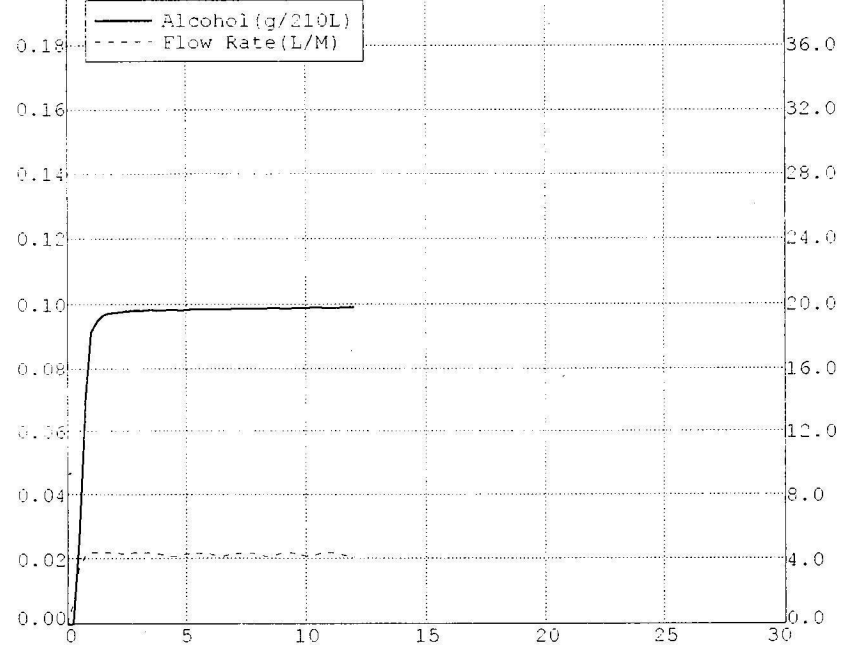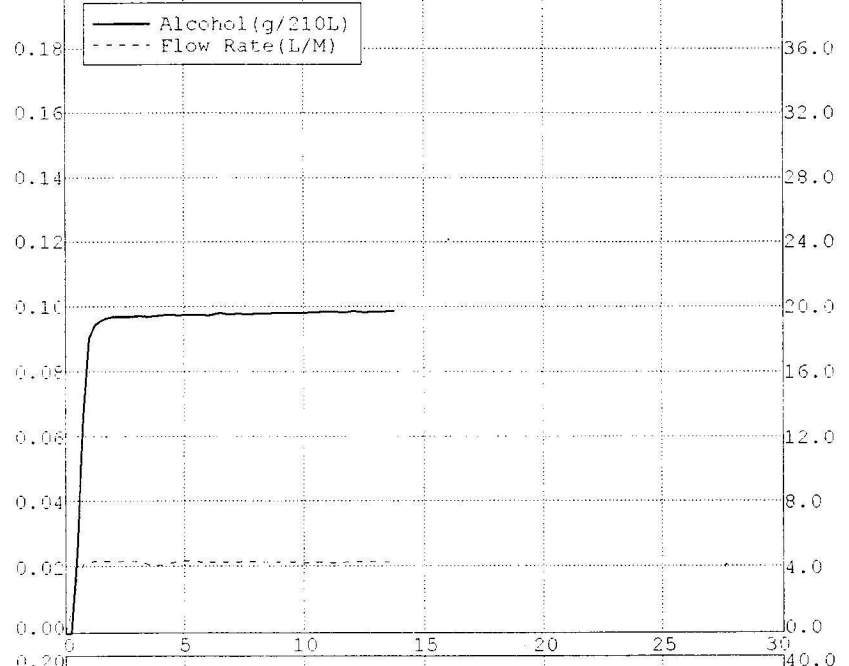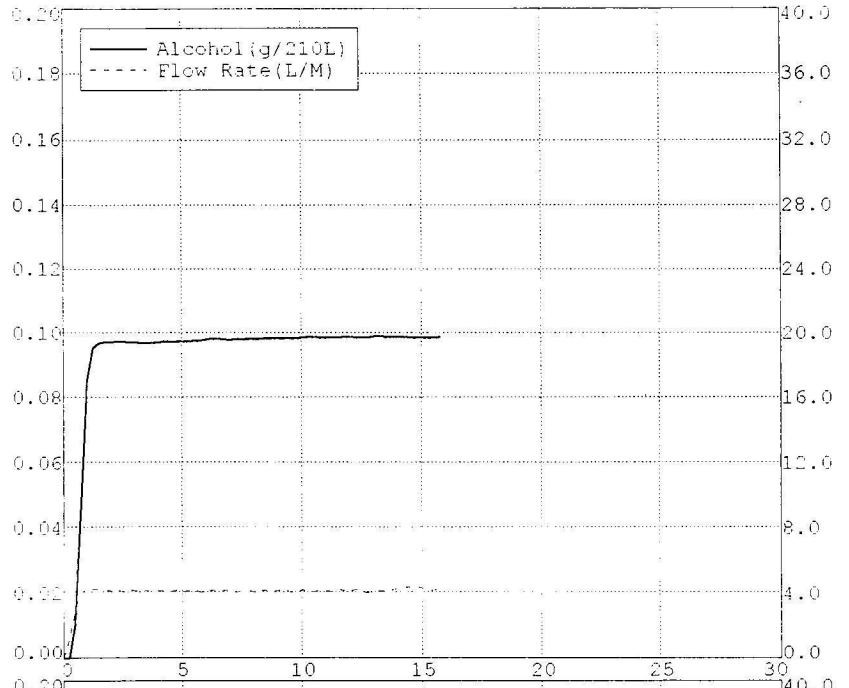

06/4