

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 06/10/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:59
INTERNAL STANDARD	VERIFIED	00:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:59
BLANK TEST	0.00	01:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:00
BLANK TEST	0.00	01:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:02
BLANK TEST	0.00	01:03

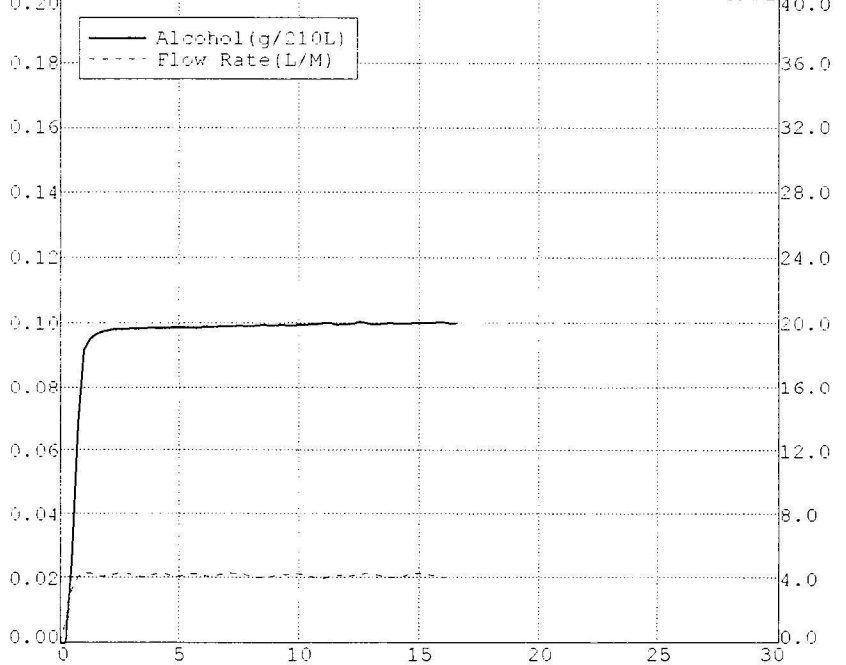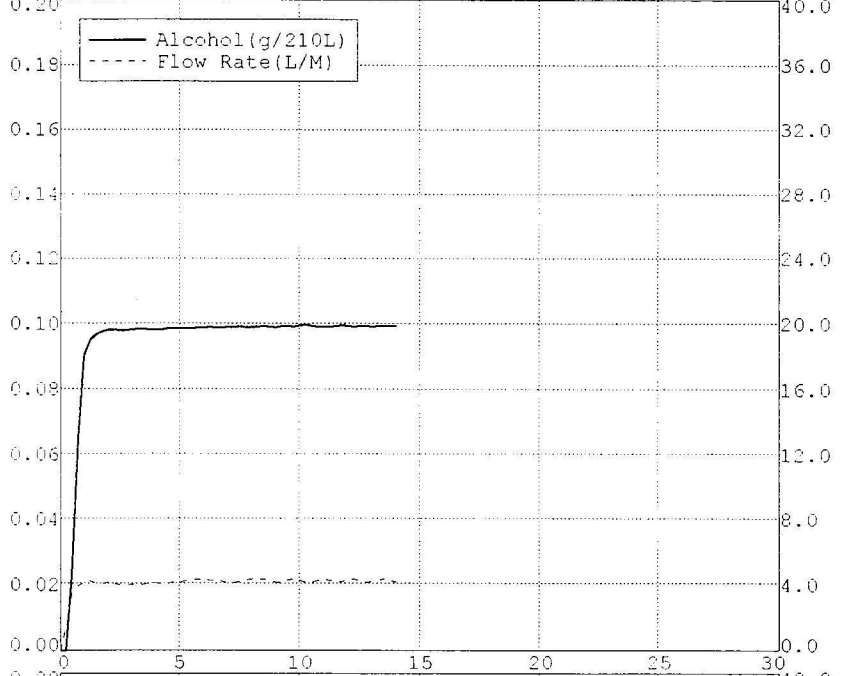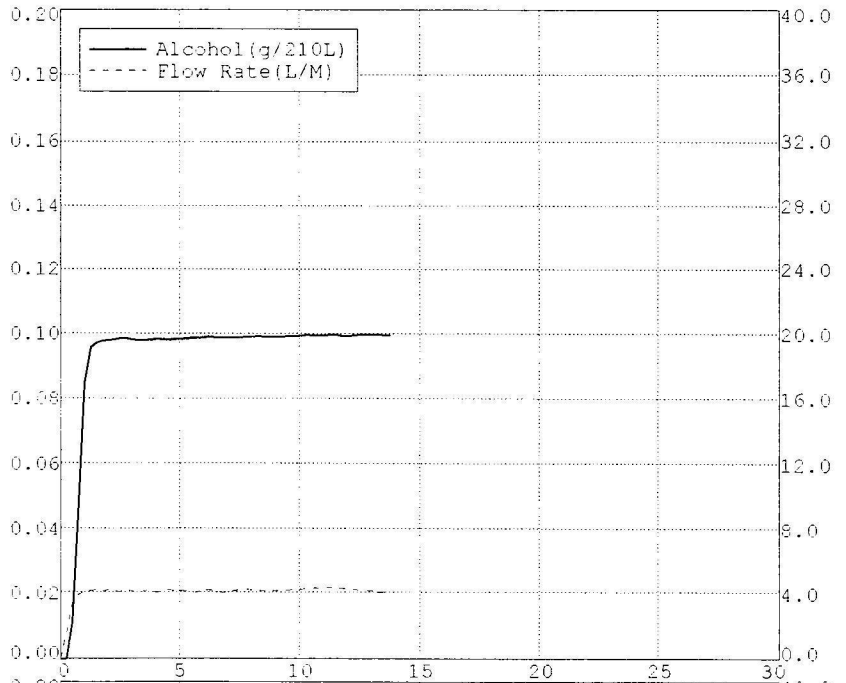

6/14