

SUPERVISOR TEST




SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 07/09/2023

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:10
INTERNAL STANDARD	VERIFIED	08:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:10
BLANK TEST	0.00	08:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:12
BLANK TEST	0.00	08:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:13
BLANK TEST	0.00	08:14

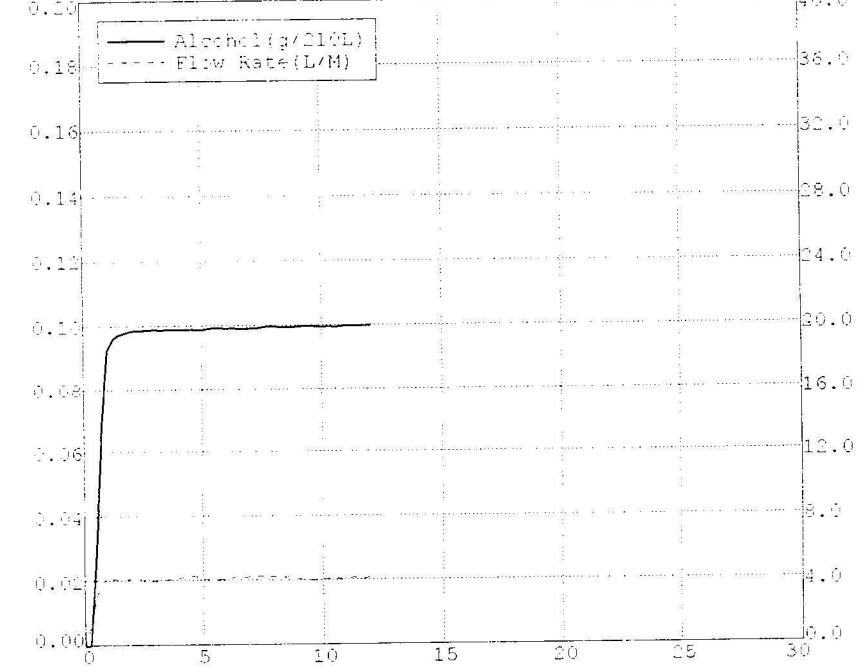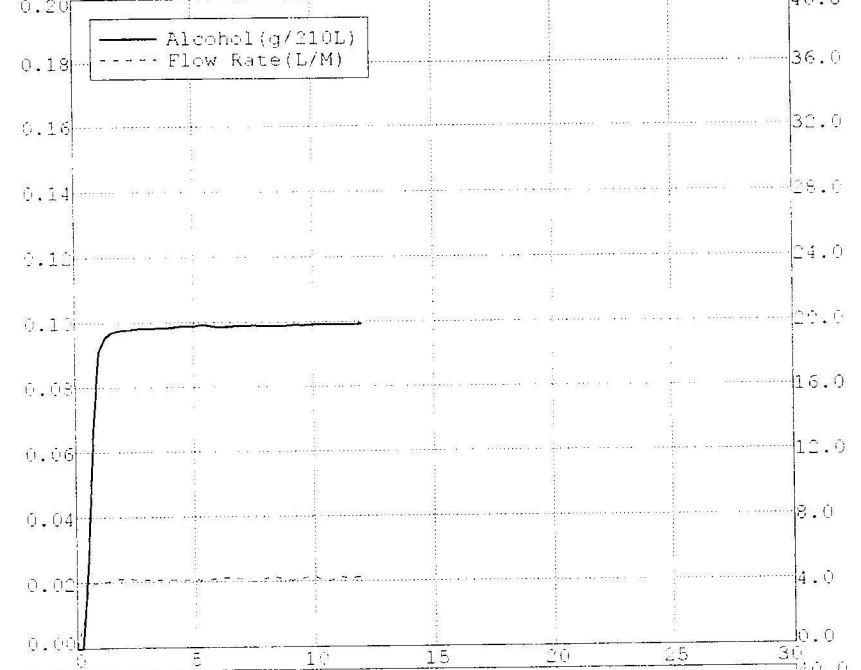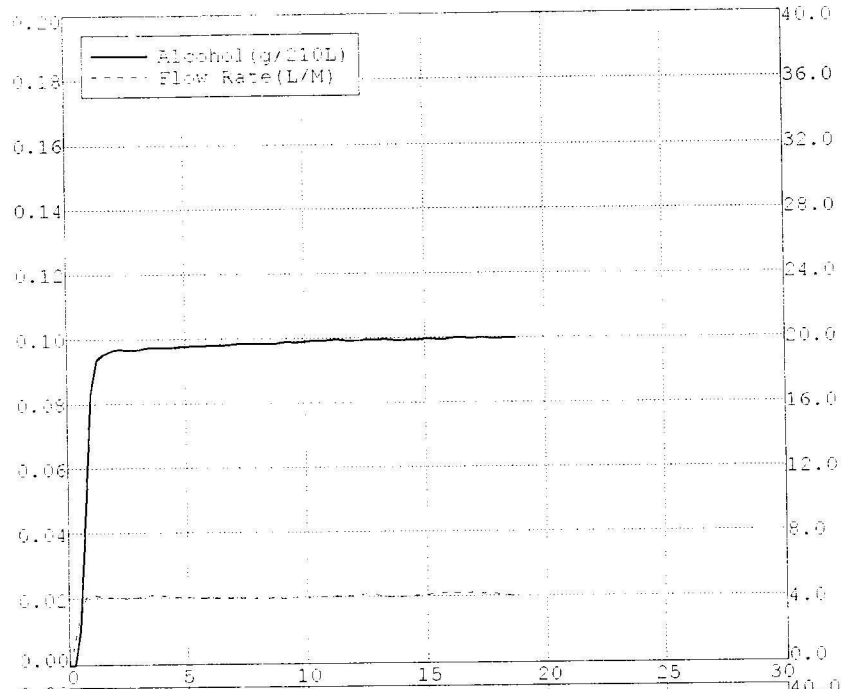

614